

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022824\
 Data File : VV034461.D
 Acq On : 28 Feb 2024 11:05
 Operator : SY/MD
 Sample : P1535-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV034461.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	84	rVB	51621	54405	9.87%	1.076%
2	1.532	146	153	167	rVB	51916	63100	11.44%	1.248%
3	2.063	305	318	333	rBV3	154057	262103	47.53%	5.186%
4	3.117	634	646	660	rBV3	6444	13692	2.48%	0.271%
5	3.815	852	863	918	rBV3	85421	289414	52.48%	5.726%
6	4.252	983	999	1029	rBV2	71479	194606	35.29%	3.850%
7	4.738	1138	1150	1166	rVB4	5126	11832	2.15%	0.234%
8	4.960	1204	1219	1248	rBV2	157933	401995	72.90%	7.954%
9	5.535	1387	1398	1424	rBV	163558	341902	62.00%	6.765%
10	5.834	1477	1491	1526	rBV	270324	551426	100.00%	10.910%
11	5.992	1528	1540	1566	rVB	91074	191981	34.82%	3.798%
12	6.918	1819	1828	1849	rBV	39669	78265	14.19%	1.549%
13	7.246	1919	1930	1952	rBV	178729	316115	57.33%	6.255%
14	7.564	2019	2029	2043	rBV	22842	42971	7.79%	0.850%
15	7.905	2117	2135	2159	rBV	248603	430531	78.08%	8.518%
16	8.027	2164	2173	2213	rBV	284669	526967	95.56%	10.426%
17	8.786	2398	2409	2437	rBV	250871	421756	76.48%	8.345%
18	10.156	2823	2835	2849	rBV	78781	124095	22.50%	2.455%
19	10.326	2878	2888	2900	rBV2	5871	9314	1.69%	0.184%
20	11.185	3145	3155	3177	rBV	264804	413775	75.04%	8.187%
21	11.561	3259	3272	3294	rBV	196948	313916	56.93%	6.211%




Sum of corrected areas: 5054161

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022824\
Data File : VV034461.D
Acq On : 28 Feb 2024 11:05
Operator : SY/MD
Sample : P1535-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

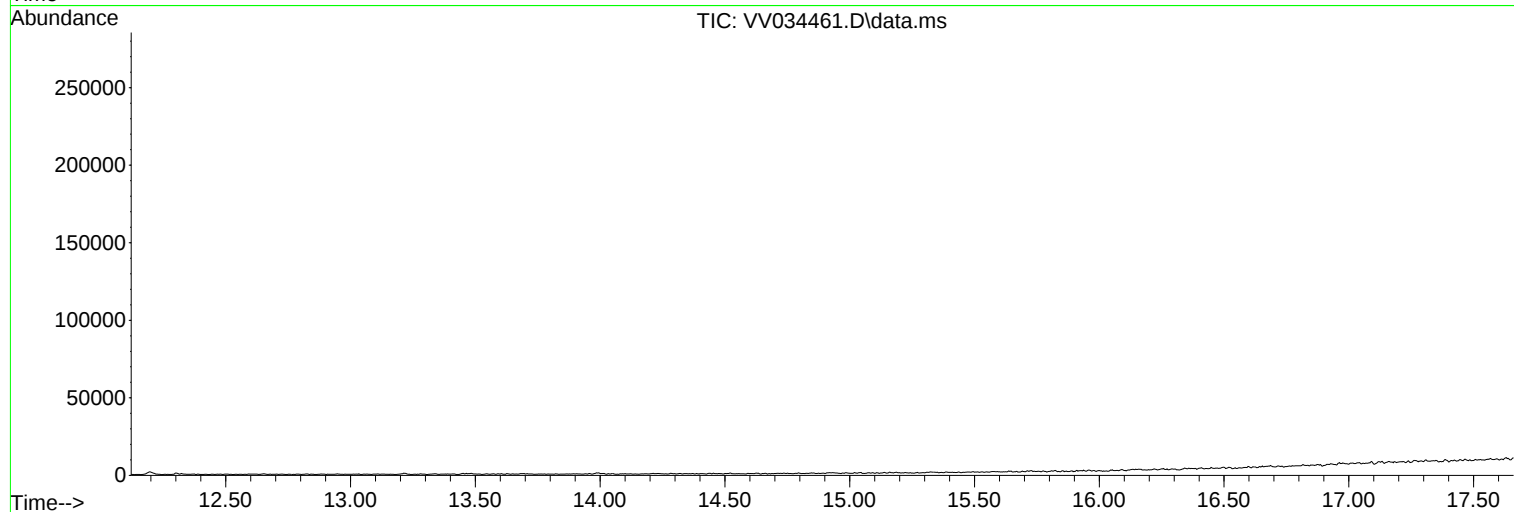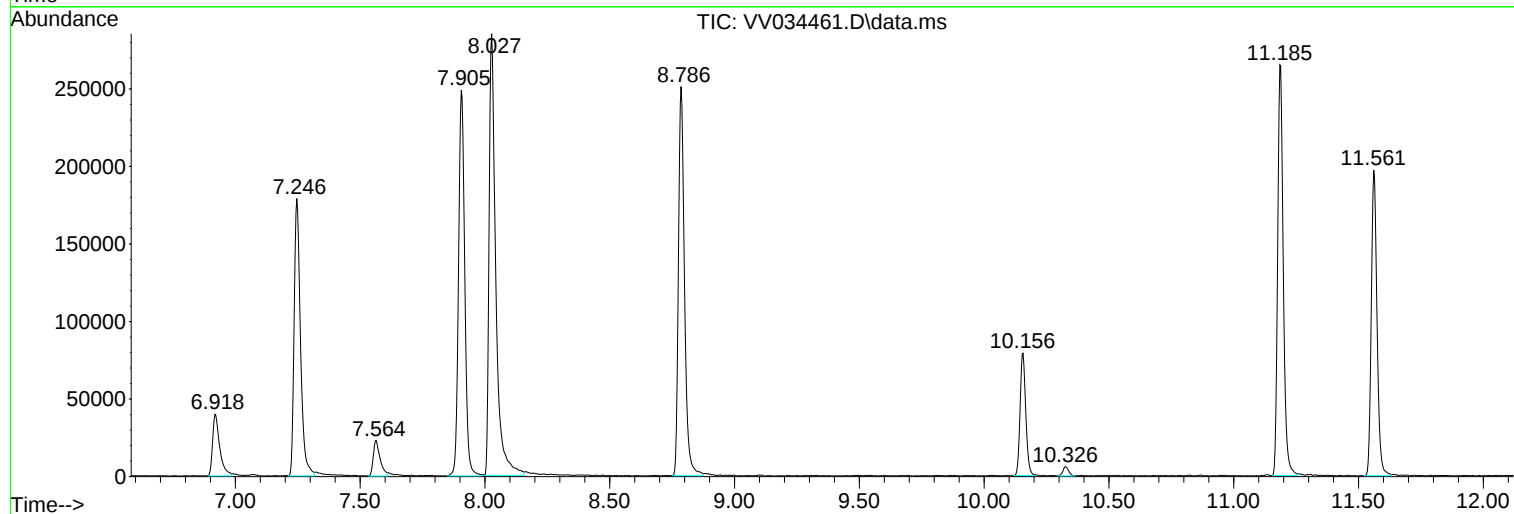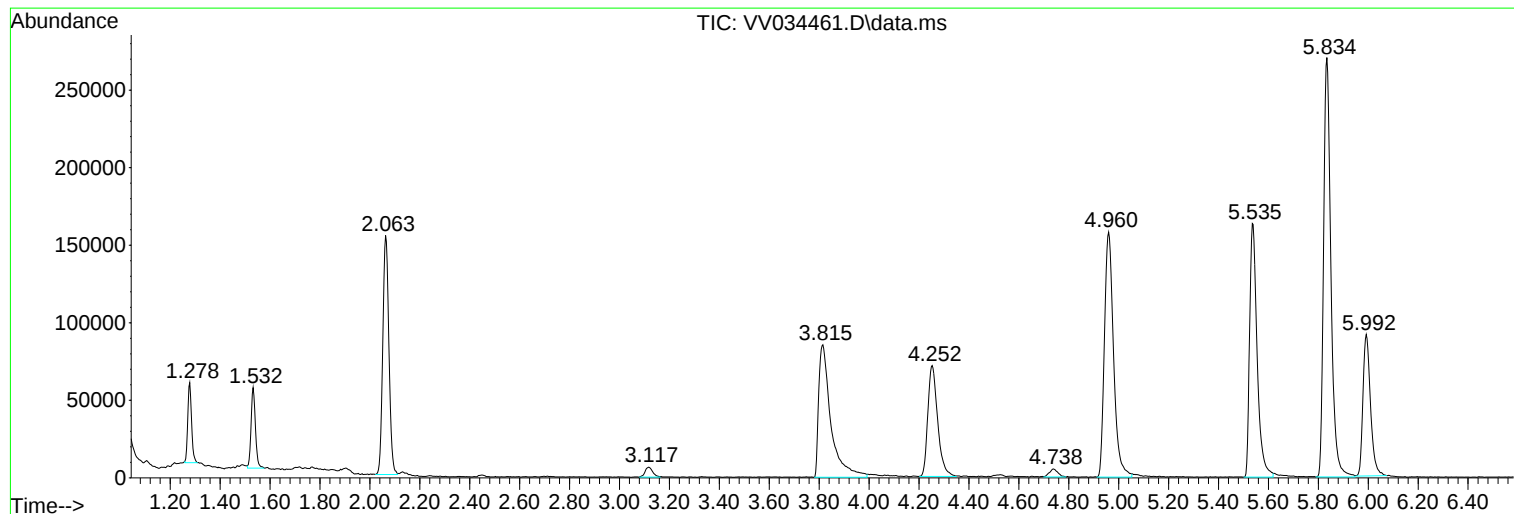

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022824\
Data File : VV034461.D
Acq On : 28 Feb 2024 11:05
Operator : SY/MD
Sample : P1535-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022824\
Data File : VV034461.D
Acq On : 28 Feb 2024 11:05
Operator : SY/MD
Sample : P1535-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------