

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022824\
 Data File : VV034462.D
 Acq On : 28 Feb 2024 11:29
 Operator : SY/MD
 Sample : P1535-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034462.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	94	rVB	55375	66756	12.14%	1.462%
2	1.532	146	153	166	rVB	53501	63821	11.60%	1.398%
3	2.060	306	317	334	rVB	98844	149383	27.16%	3.271%
4	3.825	856	866	903	rBV2	53177	214108	38.93%	4.689%
5	4.256	983	1000	1028	rBV2	77054	221382	40.25%	4.848%
6	4.735	1131	1149	1169	rBV2	26820	67123	12.21%	1.470%
7	4.960	1205	1219	1253	rBV2	163347	422045	76.74%	9.243%
8	5.535	1387	1398	1426	rBV	160817	343441	62.45%	7.521%
9	5.838	1481	1492	1518	rBV4	66552	143806	26.15%	3.149%
10	5.992	1528	1540	1568	rBV3	94542	199676	36.31%	4.373%
11	6.921	1818	1829	1849	rBV	40793	81608	14.84%	1.787%
12	7.246	1920	1930	1957	rBV	180458	326424	59.36%	7.148%
13	7.561	2018	2028	2048	rBV2	24002	47765	8.69%	1.046%
14	7.905	2115	2135	2154	rBV	204281	353184	64.22%	7.735%
15	8.027	2164	2173	2206	rBV	294372	549950	100.00%	12.044%
16	8.786	2397	2409	2437	rBV	250286	422763	76.87%	9.258%
17	10.156	2824	2835	2857	rVB	81544	130962	23.81%	2.868%
18	10.323	2878	2887	2899	rVB	10355	17138	3.12%	0.375%
19	11.188	3144	3156	3182	rBV	266738	418673	76.13%	9.169%
20	11.561	3261	3272	3293	rBV	201987	326334	59.34%	7.147%




Sum of corrected areas: 4566342

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022824\
Data File : VV034462.D
Acq On : 28 Feb 2024 11:29
Operator : SY/MD
Sample : P1535-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

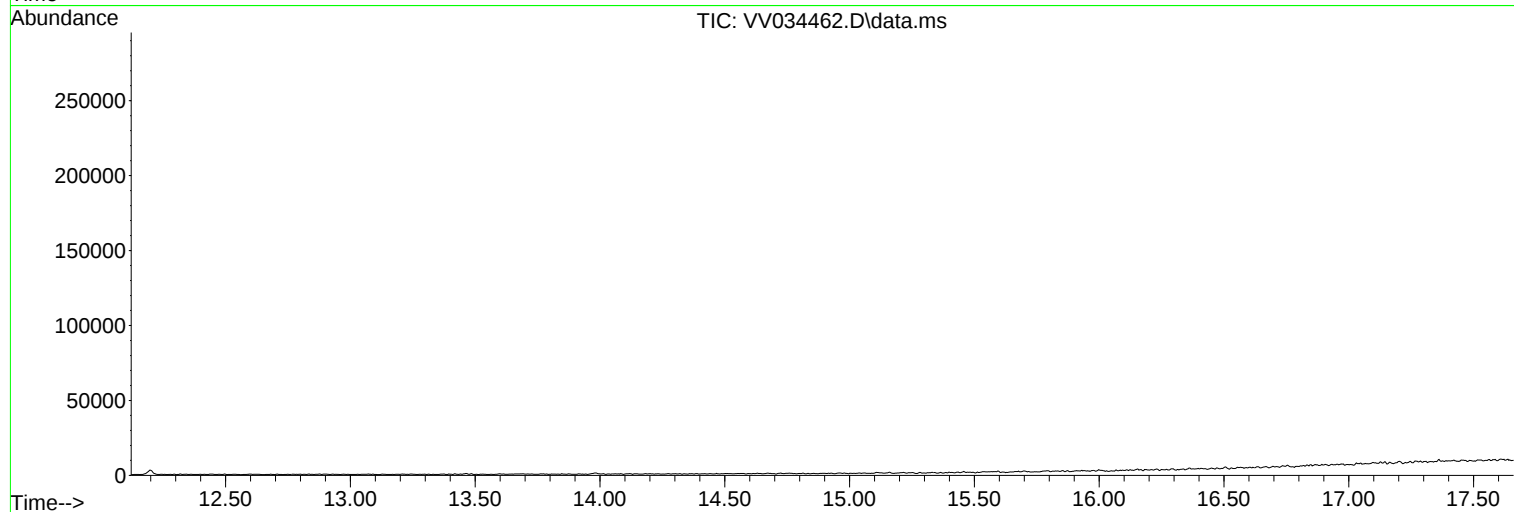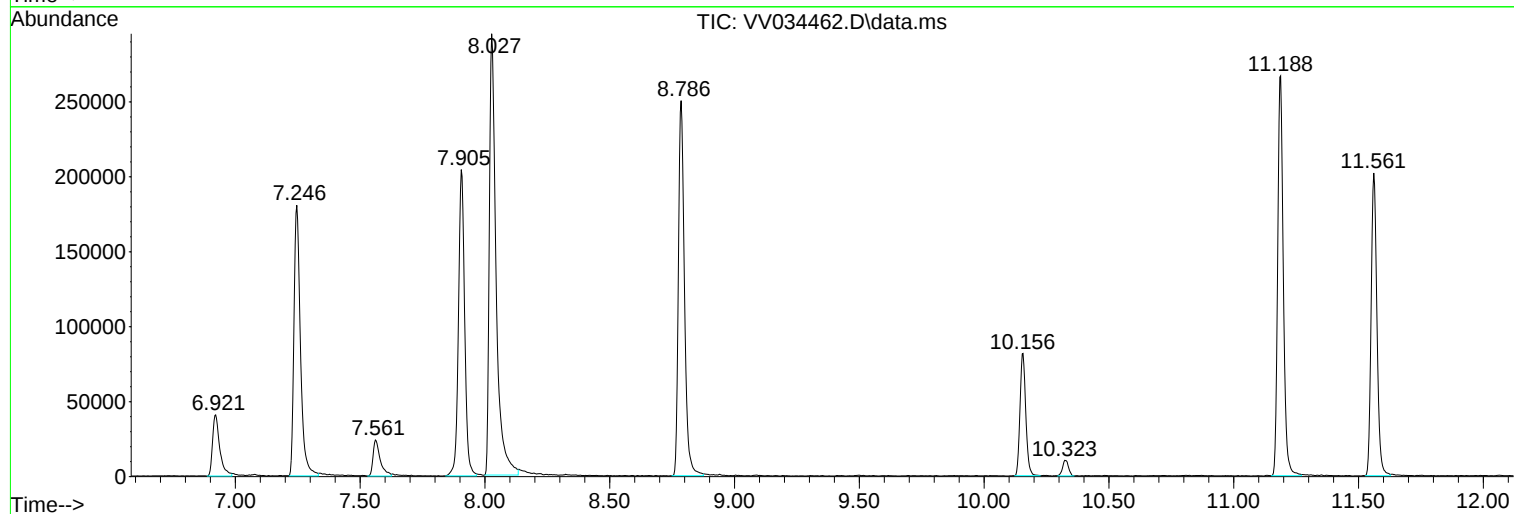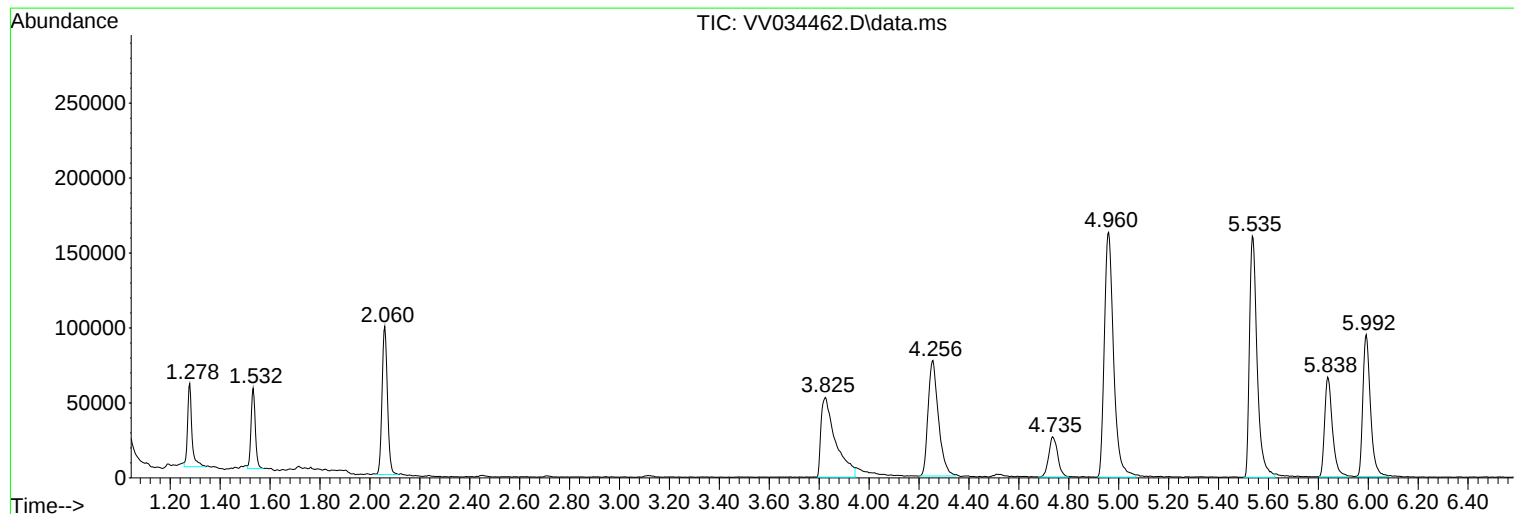

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022824\
Data File : VV034462.D
Acq On : 28 Feb 2024 11:29
Operator : SY/MD
Sample : P1535-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022824\
Data File : VV034462.D
Acq On : 28 Feb 2024 11:29
Operator : SY/MD
Sample : P1535-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc