
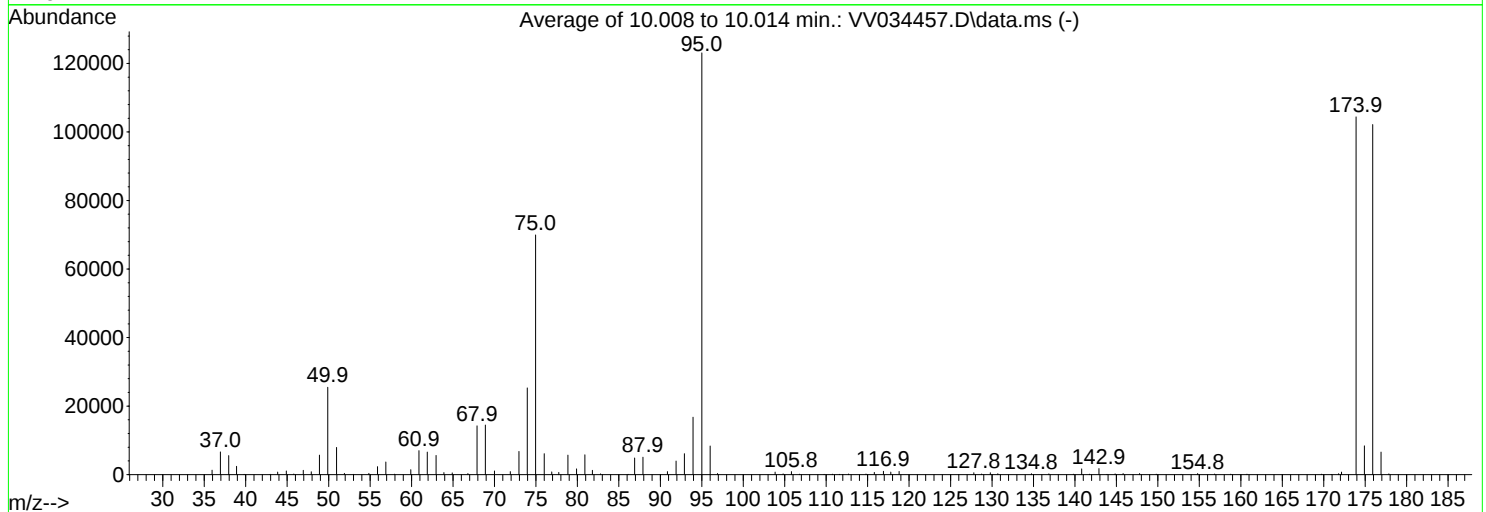


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022824\
Data File : VV034457.D
Acq On : 28 Feb 2024 08:24
Operator : SY/MD
Sample : BFB263
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB263

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Feb 29 00:34:49 2024

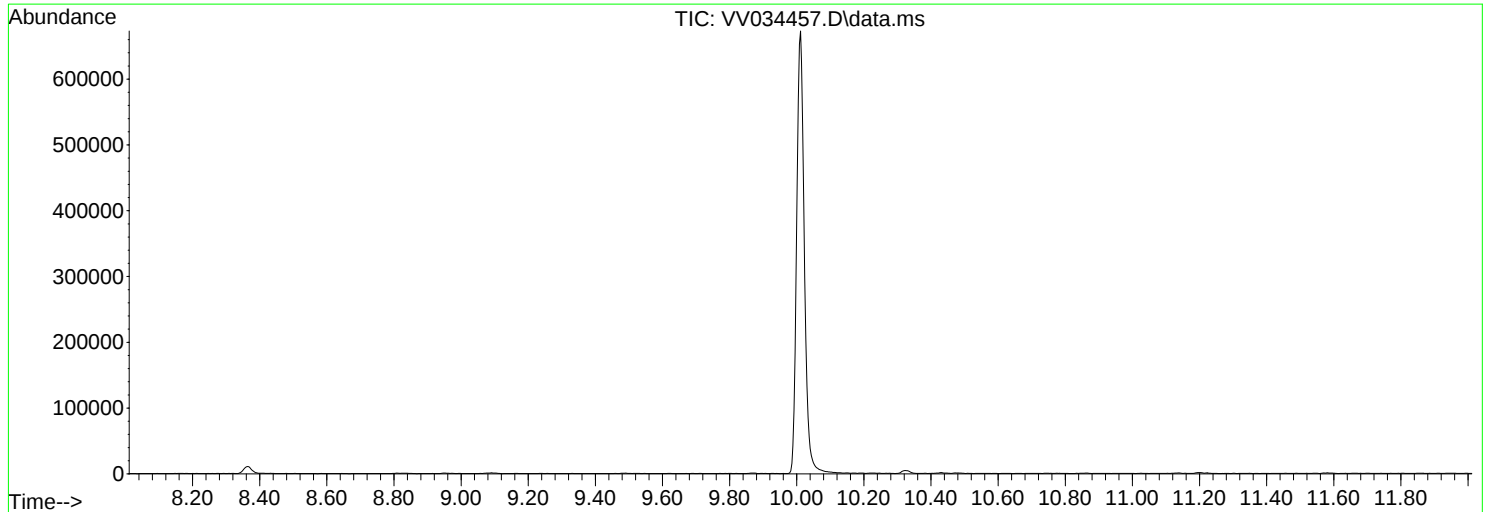

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	25483	PASS
75	95	30	80	56.8	69965	PASS
95	95	100	100	100.0	123085	PASS
96	95	5	9	6.8	8362	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.8	104403	PASS
175	174	5	9	8.1	8415	PASS
176	174	95	105	97.9	102179	PASS
177	176	5	10	6.4	6582	PASS

m/z	Abundance
39.80	253.0
43.80	313.0

Instrument :
MSVOA_V
ClientSampleId :
BFB263

m/z	Abundance
36.00	1306.0
37.00	7082.0
38.00	5897.0
38.90	2344.0
39.90	344.0
43.00	131.0
43.90	1091.0
44.90	1086.0
45.80	196.0
47.00	1279.0
47.90	889.0
48.90	5844.0
49.90	25736.0
51.00	7951.0
51.90	361.0
53.00	125.0
54.90	333.0
55.90	2383.0
56.90	3723.0
58.00	182.0
59.90	1364.0
60.90	7043.0
61.90	7005.0
63.00	5963.0
63.90	638.0
64.90	489.0
66.80	294.0
67.90	14418.0
68.90	15141.0
70.00	1004.0
71.90	895.0
72.90	6842.0
74.00	25456.0
74.90	70848.0
76.00	5866.0
76.90	770.0
77.80	652.0
78.90	5586.0
79.90	1674.0
80.90	5909.0
81.80	1366.0
82.80	259.0
86.90	4895.0
87.90	4979.0
90.80	900.0
91.90	4238.0
92.90	6090.0
93.90	17112.0
95.00	123456.0
96.00	8680.0
96.90	388.0
103.90	873.0
104.80	230.0
105.80	951.0
106.80	168.0
109.70	128.0
110.80	161.0
112.70	157.0
114.80	169.0
115.80	670.0
116.90	966.0
117.80	764.0
118.80	892.0
126.00	106.0
127.80	641.0
128.90	231.0
129.80	542.0
130.70	302.0
134.80	225.0
136.80	223.0
139.80	160.0
140.80	1777.0
141.80	149.0
142.90	1792.0
143.90	162.0
144.80	246.0
145.80	371.0
147.80	358.0
149.80	124.0
154.80	323.0
156.80	217.0
158.80	174.0
160.80	142.0
169.70	112.0
170.90	127.0
171.80	783.0
172.20	734.0
173.90	102880.0
174.90	8357.0
175.90	100288.0
176.90	6912.0
177.90	236.0

Instrument :
MSVOA_V
ClientSampleId :
BFB263

m/z	Abundance
35.90	1371.0
37.00	6903.0
38.00	5646.0
38.90	2499.0
39.80	358.0
42.90	102.0
43.90	1088.0
44.90	1164.0
45.80	208.0
46.90	1264.0
47.90	905.0
48.90	5920.0
49.90	26200.0
51.00	8203.0
51.90	379.0
53.00	101.0
54.80	355.0
55.90	2429.0
56.90	3810.0
58.00	153.0
59.90	1519.0
60.90	7261.0
61.90	6770.0
63.00	5842.0
63.90	636.0
64.90	554.0
66.80	327.0
67.90	14720.0
68.90	14892.0
70.00	1082.0
71.90	971.0
72.90	7138.0
74.00	26064.0
74.90	72536.0
76.00	6393.0
76.90	871.0
77.70	698.0
78.90	5917.0
79.90	1757.0
80.90	5930.0
81.80	1312.0
82.80	224.0
86.10	158.0
86.90	5020.0
87.90	5337.0
90.80	915.0
91.90	4095.0
92.90	6292.0
94.00	17280.0
95.00	127296.0
96.00	8597.0
96.90	362.0
103.80	789.0
104.80	251.0
105.80	915.0
106.80	165.0
109.70	120.0
110.70	163.0
111.60	111.0
112.70	191.0
114.80	176.0
115.80	720.0
116.90	1039.0
117.80	816.0
118.80	950.0
127.80	585.0
128.70	203.0
129.80	569.0
130.70	312.0
134.70	251.0
136.90	257.0
139.80	161.0
140.80	1734.0
141.70	149.0
142.90	1832.0
143.80	132.0
144.80	226.0
145.80	355.0
147.80	342.0
149.80	137.0
152.80	104.0
154.80	333.0
156.80	203.0
158.80	162.0
160.70	141.0
169.70	141.0
172.10	789.0
173.90	107872.0
174.90	8747.0
175.90	106160.0
176.90	6849.0
177.80	216.0

Instrument :
MSVOA_V
ClientSampleId :
BFB263

m/z	Abundance
35.90	1254.0
36.90	5951.0
37.90	5121.0
38.90	2484.0
39.80	341.0
43.90	1068.0
44.90	1040.0
45.80	145.0
46.90	1283.0
47.90	808.0
48.90	5284.0
49.90	24512.0
50.90	7633.0
51.90	365.0
54.80	385.0
55.90	2260.0
56.90	3584.0
57.90	119.0
59.90	1428.0
60.90	6716.0
61.90	5975.0
62.90	5044.0
63.90	578.0
64.90	566.0
66.80	349.0
67.90	13580.0
68.90	13445.0
70.00	1086.0
71.90	827.0
73.00	6344.0
73.90	24376.0
75.00	66512.0
76.00	6052.0
76.90	802.0
77.70	580.0
78.80	5560.0
79.90	1612.0
80.90	5493.0
81.80	1182.0
82.80	178.0
86.10	107.0
86.90	4671.0
87.90	4995.0
90.90	815.0
91.90	3642.0
92.90	5982.0
94.00	15929.0
95.00	118504.0
96.00	7809.0
96.90	257.0
103.80	624.0
104.80	240.0
105.80	757.0
106.80	162.0
109.80	103.0
110.70	166.0
111.60	113.0
112.00	116.0
112.70	195.0
114.80	181.0
115.80	632.0
116.90	997.0
117.80	699.0
118.80	897.0
127.80	488.0
128.70	175.0
129.80	565.0
130.70	231.0
134.70	317.0
136.90	277.0
139.80	136.0
140.80	1471.0
141.70	162.0
142.90	1664.0
144.90	209.0
145.80	278.0
147.80	323.0
149.80	131.0
152.80	117.0
154.80	332.0
156.90	172.0
158.80	150.0
160.70	144.0
169.80	145.0
172.10	705.0
173.90	102456.0
174.90	8141.0
175.90	100088.0
176.90	5984.0
177.80	190.0

Instrument :
MSVOA_V
ClientSampleId :
BFB263