

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
 Data File : VV034475.D
 Acq On : 29 Feb 2024 12:34
 Operator : SY/MD
 Sample : VV0229MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK232

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034475.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	197792	209434	15.92%	2.133%
2	1.529	145	152	166	rVB	165177	197166	14.99%	2.008%
3	2.056	306	316	334	rBV	333526	490897	37.31%	5.000%
4	2.449	430	438	451	rVB3	4596	7926	0.60%	0.081%
5	2.497	451	453	456	rBV	171	108	0.01%	0.001%
6	2.693	511	514	515	rBV2	461	259	0.02%	0.003%
7	2.744	526	530	535	rBV2	253	225	0.02%	0.002%
8	2.867	564	568	571	rBV	221	187	0.01%	0.002%
9	2.912	580	582	585	rBV	223	82	0.01%	0.001%
10	2.989	602	606	609	rBV2	154	148	0.01%	0.002%
11	3.005	609	611	615	rVB	272	147	0.01%	0.001%
12	3.040	619	622	627	rBV2	212	187	0.01%	0.002%
13	3.088	635	637	644	rVB2	280	205	0.02%	0.002%
14	3.156	655	658	660	rBV	185	135	0.01%	0.001%
15	3.201	669	672	674	rBV2	139	112	0.01%	0.001%
16	3.233	679	682	687	rVB	184	148	0.01%	0.002%
17	3.297	696	702	704	rBV	218	153	0.01%	0.002%
18	3.326	709	711	713	rVV2	217	108	0.01%	0.001%
19	3.355	716	720	723	rVB2	326	251	0.02%	0.003%
20	3.384	723	729	732	rBV	273	255	0.02%	0.003%
21	3.481	756	759	761	rBV2	175	104	0.01%	0.001%
22	3.593	788	794	802	rVB2	217	281	0.02%	0.003%
23	3.712	827	831	833	rBV2	258	172	0.01%	0.002%
24	3.786	845	854	882	rBV	106257	285435	21.70%	2.907%
25	4.249	982	998	1024	rBV	206621	531965	40.44%	5.418%
26	4.539	1086	1088	1090	rBV2	466	280	0.02%	0.003%
27	4.638	1116	1119	1123	rVB3	419	367	0.03%	0.004%
28	4.664	1123	1127	1129	rBV2	327	250	0.02%	0.003%
29	4.696	1135	1137	1141	rBV2	279	208	0.02%	0.002%
30	4.715	1141	1143	1148	rVB2	241	166	0.01%	0.002%
31	4.802	1167	1170	1172	rBV	156	109	0.01%	0.001%
32	4.953	1201	1217	1254	rBV2	500681	1315584	100.00%	13.400%
33	5.323	1330	1332	1334	rBV2	281	142	0.01%	0.001%
34	5.461	1373	1375	1380	rBV3	334	206	0.02%	0.002%
35	5.532	1386	1397	1426	rBV	356118	733866	55.78%	7.475%
36	5.834	1480	1491	1511	rVB3	11167	25493	1.94%	0.260%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
 Data File : VV034475.D
 Acq On : 29 Feb 2024 12:34
 Operator : SY/MD
 Sample : VV0229MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK232

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	5.918	1516	1517	1518	rBV3	239	83	0.01%	0.001%
38	5.989	1526	1539	1571	rBV	283083	593623	45.12%	6.046%
39	6.198	1602	1604	1607	rBV3	317	205	0.02%	0.002%
40	6.217	1608	1610	1616	rVB3	417	296	0.02%	0.003%
41	6.243	1616	1618	1619	rBV3	409	156	0.01%	0.002%
42	6.336	1644	1647	1651	rBV2	133	137	0.01%	0.001%
43	6.358	1651	1654	1657	rVB	267	121	0.01%	0.001%
44	6.436	1675	1678	1679	rBV	182	102	0.01%	0.001%
45	6.481	1687	1692	1697	rBV2	203	234	0.02%	0.002%
46	6.567	1716	1719	1720	rBV	158	78	0.01%	0.001%
47	6.735	1769	1771	1773	rBV2	170	88	0.01%	0.001%
48	6.757	1776	1778	1782	rVV2	248	182	0.01%	0.002%
49	6.802	1790	1792	1798	rBV2	294	163	0.01%	0.002%
50	6.911	1815	1826	1854	rBV	150773	285075	21.67%	2.904%
51	7.130	1891	1894	1896	rBV2	553	411	0.03%	0.004%
52	7.198	1913	1915	1917	rBV	218	95	0.01%	0.001%
53	7.243	1917	1929	1962	rBV	581650	1023919	77.83%	10.429%
54	7.555	2017	2026	2052	rBV	99694	187282	14.24%	1.908%
55	7.809	2103	2105	2109	rVB2	355	221	0.02%	0.002%
56	7.860	2118	2121	2123	rBV2	518	327	0.02%	0.003%
57	7.911	2134	2137	2140	rVB3	465	340	0.03%	0.003%
58	7.944	2146	2147	2150	rVB	386	94	0.01%	0.001%
59	8.024	2162	2172	2210	rBV	393170	701355	53.31%	7.143%
60	8.590	2345	2348	2353	rBB2	348	278	0.02%	0.003%
61	8.616	2353	2356	2359	rBV2	368	239	0.02%	0.002%
62	8.667	2370	2372	2375	rBV3	157	115	0.01%	0.001%
63	8.741	2393	2395	2398	rVB2	325	197	0.01%	0.002%
64	8.783	2398	2408	2442	rBV	536962	874900	66.50%	8.911%
65	9.085	2499	2502	2503	rBV	333	189	0.01%	0.002%
66	9.178	2528	2531	2537	rBV2	145	147	0.01%	0.001%
67	9.297	2565	2568	2571	rBV2	315	222	0.02%	0.002%
68	9.423	2603	2607	2609	rBV	259	207	0.02%	0.002%
69	9.497	2626	2630	2634	rVB3	429	374	0.03%	0.004%
70	9.516	2634	2636	2638	rBV2	185	103	0.01%	0.001%
71	9.538	2641	2643	2644	rBV	278	100	0.01%	0.001%
72	9.583	2652	2657	2660	rBV2	251	237	0.02%	0.002%
73	9.673	2683	2685	2687	rBV	228	98	0.01%	0.001%
74	9.715	2694	2698	2700	rBV	184	137	0.01%	0.001%
75	9.754	2707	2710	2713	rBV	178	120	0.01%	0.001%
76	9.870	2741	2746	2754	rVV2	402	517	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
 Data File : VV034475.D
 Acq On : 29 Feb 2024 12:34
 Operator : SY/MD
 Sample : VV0229MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK232

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	9.947	2767	2770	2771	rBV	272	126	0.01%	0.001%
78	10.027	2792	2795	2798	rBV2	271	193	0.01%	0.002%
79	10.040	2798	2799	2801	rVB	221	86	0.01%	0.001%
80	10.107	2817	2820	2822	rBV	177	107	0.01%	0.001%
81	10.152	2822	2834	2855	rBV	376637	590941	44.92%	6.019%
82	10.368	2898	2901	2906	rBV	187	182	0.01%	0.002%
83	10.416	2913	2916	2922	rVB2	165	161	0.01%	0.002%
84	10.445	2922	2925	2927	rBV2	264	172	0.01%	0.002%
85	10.770	3023	3026	3031	rBV	205	183	0.01%	0.002%
86	10.866	3050	3056	3060	rBV3	828	935	0.07%	0.010%
87	11.124	3132	3136	3138	rBV3	929	657	0.05%	0.007%
88	11.185	3144	3155	3178	rBV	537317	827199	62.88%	8.425%
89	11.561	3260	3272	3294	rBV	570542	904581	68.76%	9.213%
90	11.908	3377	3380	3381	rBV	199	104	0.01%	0.001%
91	11.943	3389	3391	3394	rBV	177	123	0.01%	0.001%
92	12.586	3586	3591	3593	rBV3	926	882	0.07%	0.009%
93	12.786	3650	3653	3656	rVB2	236	146	0.01%	0.001%
94	12.876	3679	3681	3684	rBV2	225	133	0.01%	0.001%
95	13.204	3778	3783	3784	rBV4	2040	1521	0.12%	0.015%
96	13.310	3814	3816	3819	rVB	353	166	0.01%	0.002%
97	13.336	3821	3824	3827	rBV2	394	274	0.02%	0.003%
98	13.451	3852	3860	3870	rVB2	5566	8706	0.66%	0.089%
99	13.657	3920	3924	3926	rBV3	487	383	0.03%	0.004%
100	13.686	3926	3933	3945	rVB3	2962	4655	0.35%	0.047%




Sum of corrected areas: 9818144

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
Data File : VV034475.D
Acq On : 29 Feb 2024 12:34
Operator : SY/MD
Sample : VV0229MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK232

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

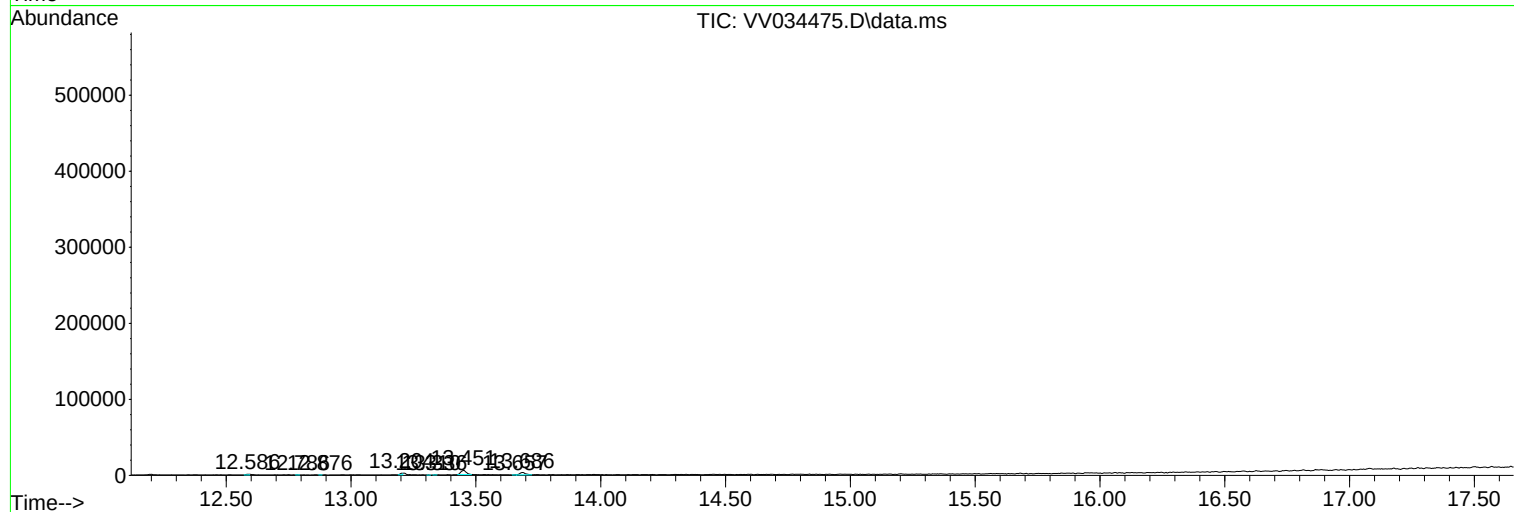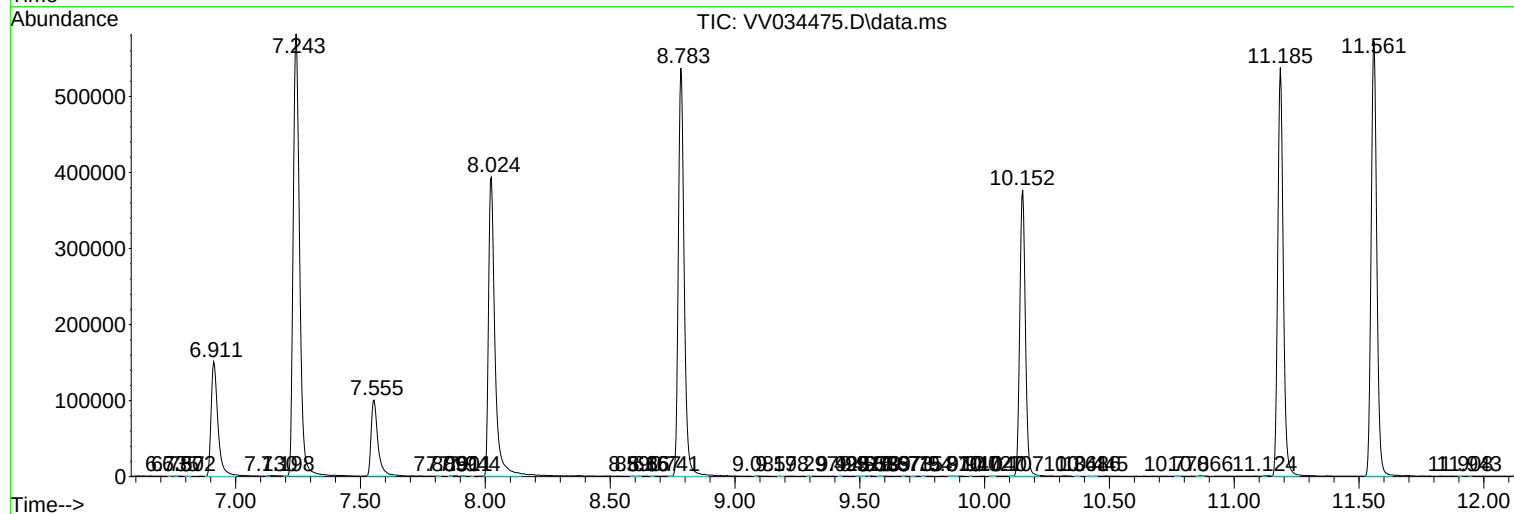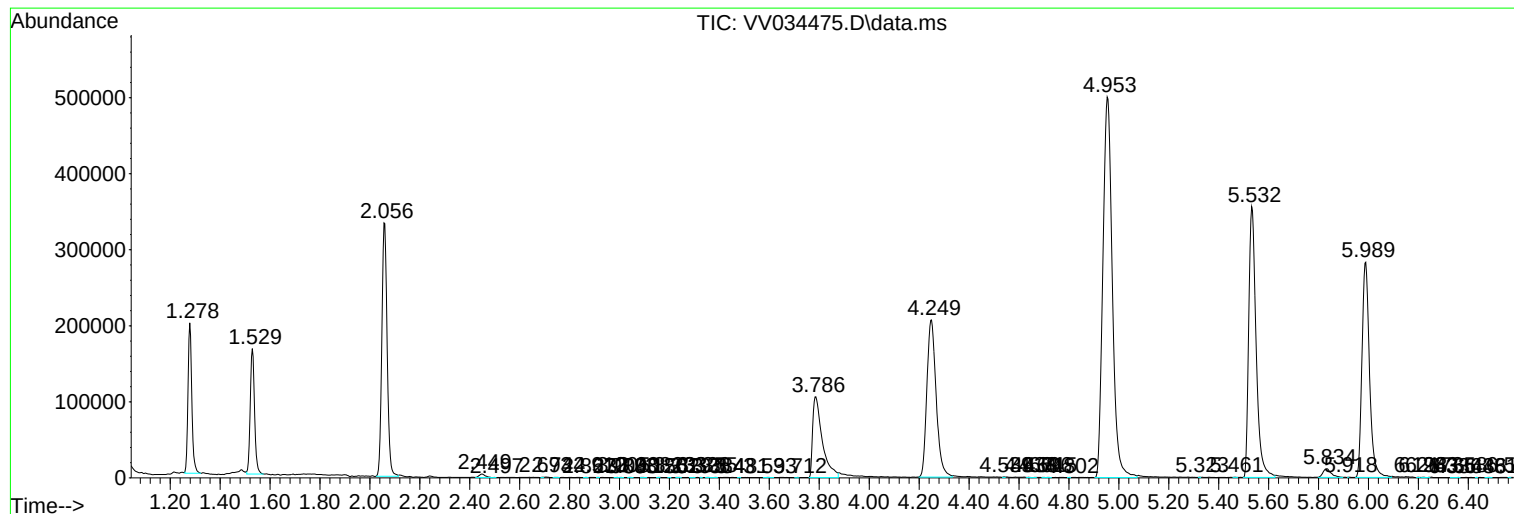

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
Data File : VV034475.D
Acq On : 29 Feb 2024 12:34
Operator : SY/MD
Sample : VV0229MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK232

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
Data File : VV034475.D
Acq On : 29 Feb 2024 12:34
Operator : SY/MD
Sample : VV0229MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK232

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc