

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
 Data File : VV034476.D
 Acq On : 29 Feb 2024 12:58
 Operator : SY/MD
 Sample : VV0229WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK233

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034476.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	94	rVB	194347	205723	15.85%	2.114%
2	1.529	145	152	169	rVB	163519	193592	14.91%	1.989%
3	2.059	306	317	332	rBV	324091	482384	37.16%	4.957%
4	2.449	430	438	448	rBV3	4971	7872	0.61%	0.081%
5	2.699	513	516	518	rBV3	542	379	0.03%	0.004%
6	2.879	569	572	574	rBV	155	92	0.01%	0.001%
7	3.021	614	616	617	rVB	218	79	0.01%	0.001%
8	3.059	625	628	630	rBV2	140	86	0.01%	0.001%
9	3.130	647	650	651	rBV	144	84	0.01%	0.001%
10	3.275	691	695	698	rBV2	256	234	0.02%	0.002%
11	3.349	715	718	725	rVB2	172	181	0.01%	0.002%
12	3.384	725	729	732	rBV2	199	211	0.02%	0.002%
13	3.429	739	743	748	rBV2	272	297	0.02%	0.003%
14	3.455	749	751	754	rVB2	217	111	0.01%	0.001%
15	3.516	766	770	774	rVB2	187	159	0.01%	0.002%
16	3.561	781	784	786	rBV2	199	130	0.01%	0.001%
17	3.590	791	793	796	rBV2	135	75	0.01%	0.001%
18	3.609	796	799	802	rBV	147	108	0.01%	0.001%
19	3.641	808	809	813	rBV2	182	112	0.01%	0.001%
20	3.748	837	842	845	rBV2	210	141	0.01%	0.001%
21	3.786	845	854	900	rBV	109054	302265	23.28%	3.106%
22	4.194	978	981	982	rBV2	312	179	0.01%	0.002%
23	4.249	982	998	1028	rVV	205018	526798	40.58%	5.414%
24	4.712	1140	1142	1145	rBV2	203	82	0.01%	0.001%
25	4.747	1151	1153	1155	rBV2	195	111	0.01%	0.001%
26	4.786	1164	1165	1170	rVB	146	77	0.01%	0.001%
27	4.847	1180	1184	1186	rBV2	168	121	0.01%	0.001%
28	4.860	1186	1188	1191	rBV2	211	131	0.01%	0.001%
29	4.953	1201	1217	1257	rBV2	491964	1298142	100.00%	13.340%
30	5.407	1356	1358	1361	rVB	458	266	0.02%	0.003%
31	5.423	1361	1363	1364	rVV	181	75	0.01%	0.001%
32	5.432	1364	1366	1376	rVB3	322	401	0.03%	0.004%
33	5.532	1386	1397	1433	rBV	351194	723397	55.73%	7.434%
34	5.831	1480	1490	1513	rVB4	11747	26429	2.04%	0.272%
35	5.915	1513	1516	1518	rBV2	232	121	0.01%	0.001%
36	5.989	1525	1539	1568	rBV	279360	579724	44.66%	5.957%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
 Data File : VV034476.D
 Acq On : 29 Feb 2024 12:58
 Operator : SY/MD
 Sample : VV0229WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK233

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.217	1608	1610	1613	rBV2	417	235	0.02%	0.002%
38	6.320	1638	1642	1643	rBV	312	180	0.01%	0.002%
39	6.345	1646	1650	1652	rBB2	254	152	0.01%	0.002%
40	6.362	1652	1655	1657	rBV2	180	117	0.01%	0.001%
41	6.403	1665	1668	1674	rVB	237	147	0.01%	0.002%
42	6.442	1677	1680	1683	rVB	310	183	0.01%	0.002%
43	6.458	1683	1685	1688	rBV	175	112	0.01%	0.001%
44	6.497	1694	1697	1699	rBV2	116	77	0.01%	0.001%
45	6.558	1713	1716	1718	rBV	128	89	0.01%	0.001%
46	6.587	1722	1725	1728	rBV2	462	393	0.03%	0.004%
47	6.699	1758	1760	1763	rVB	223	107	0.01%	0.001%
48	6.718	1763	1766	1770	rBV2	393	273	0.02%	0.003%
49	6.741	1770	1773	1776	rBV2	197	157	0.01%	0.002%
50	6.776	1781	1784	1786	rBV2	359	177	0.01%	0.002%
51	6.799	1790	1791	1796	rBV2	155	122	0.01%	0.001%
52	6.911	1816	1826	1850	rBV	148903	279759	21.55%	2.875%
53	7.243	1918	1929	1958	rBV	572844	1008859	77.72%	10.367%
54	7.554	2016	2026	2054	rBV	101091	186383	14.36%	1.915%
55	7.825	2108	2110	2117	rVB3	465	371	0.03%	0.004%
56	7.857	2117	2120	2121	rBV	303	210	0.02%	0.002%
57	7.918	2137	2139	2142	rVB2	467	173	0.01%	0.002%
58	8.024	2162	2172	2199	rBV	406273	704879	54.30%	7.244%
59	8.558	2336	2338	2340	rBV	244	120	0.01%	0.001%
60	8.628	2357	2360	2364	rBV2	229	202	0.02%	0.002%
61	8.783	2397	2408	2442	rBV	522441	864445	66.59%	8.883%
62	9.014	2477	2480	2482	rBV2	516	268	0.02%	0.003%
63	9.075	2496	2499	2502	rBV2	238	170	0.01%	0.002%
64	9.095	2502	2505	2507	rBV3	531	365	0.03%	0.004%
65	9.149	2519	2522	2524	rBV	149	98	0.01%	0.001%
66	9.278	2560	2562	2563	rBV	190	83	0.01%	0.001%
67	9.419	2600	2606	2610	rVB2	293	287	0.02%	0.003%
68	9.468	2618	2621	2624	rBV2	151	114	0.01%	0.001%
69	9.574	2651	2654	2656	rBV	178	93	0.01%	0.001%
70	9.648	2673	2677	2680	rBV	256	223	0.02%	0.002%
71	9.709	2691	2696	2703	rBV3	377	404	0.03%	0.004%
72	9.767	2711	2714	2717	rBV2	226	135	0.01%	0.001%
73	9.795	2717	2723	2724	rBV2	186	165	0.01%	0.002%
74	9.879	2745	2749	2750	rBV2	391	285	0.02%	0.003%
75	9.927	2761	2764	2769	rBV	182	156	0.01%	0.002%
76	10.066	2805	2807	2810	rVB2	292	142	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
 Data File : VV034476.D
 Acq On : 29 Feb 2024 12:58
 Operator : SY/MD
 Sample : VV0229WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK233

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.152	2822	2834	2857	rBV	372419	590652	45.50%	6.070%
78	10.384	2903	2906	2907	rBV2	163	92	0.01%	0.001%
79	10.474	2931	2934	2937	rBV3	488	297	0.02%	0.003%
80	10.644	2982	2987	2991	rBV	241	231	0.02%	0.002%
81	10.667	2991	2994	3002	rVV	317	351	0.03%	0.004%
82	10.821	3039	3042	3045	rBV	199	141	0.01%	0.001%
83	10.918	3069	3072	3076	rVB	365	237	0.02%	0.002%
84	11.185	3144	3155	3176	rBV	529525	824887	63.54%	8.477%
85	11.422	3226	3229	3236	rVB2	435	461	0.04%	0.005%
86	11.458	3236	3240	3243	rBV	247	228	0.02%	0.002%
87	11.561	3260	3272	3291	rBV	567749	899119	69.26%	9.240%
88	11.770	3334	3337	3339	rBV2	381	158	0.01%	0.002%
89	11.783	3339	3341	3345	rBV2	195	116	0.01%	0.001%
90	11.828	3354	3355	3359	rBV2	161	75	0.01%	0.001%
91	12.188	3463	3467	3468	rBV2	583	445	0.03%	0.005%
92	12.596	3587	3594	3598	rBV5	522	617	0.05%	0.006%
93	12.763	3643	3646	3648	rBV2	250	126	0.01%	0.001%
94	12.834	3666	3668	3671	rBV2	258	167	0.01%	0.002%
95	12.895	3685	3687	3688	rBV2	197	78	0.01%	0.001%
96	12.934	3697	3699	3701	rBV	285	121	0.01%	0.001%
97	13.210	3779	3785	3800	rVB6	2048	2954	0.23%	0.030%
98	13.451	3854	3860	3871	rVB3	3438	4947	0.38%	0.051%
99	13.538	3883	3887	3888	rBV2	245	200	0.02%	0.002%
100	13.692	3927	3935	3943	rBV4	1941	3110	0.24%	0.032%




Sum of corrected areas: 9731089

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
Data File : VV034476.D
Acq On : 29 Feb 2024 12:58
Operator : SY/MD
Sample : VV0229WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK233

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

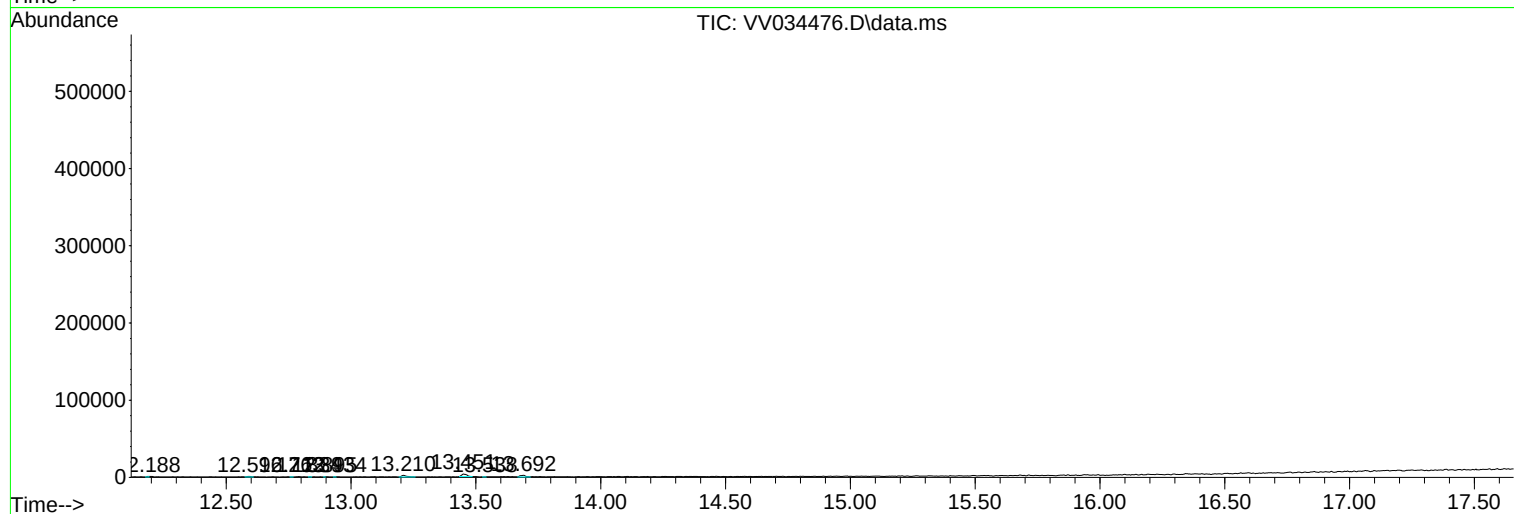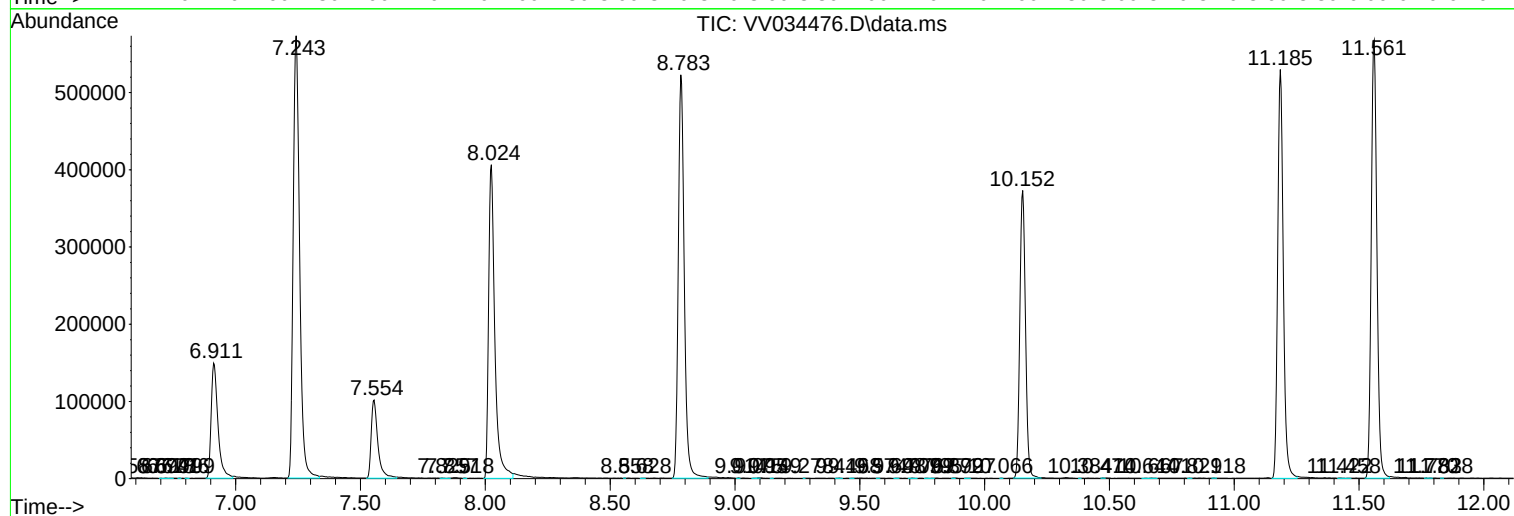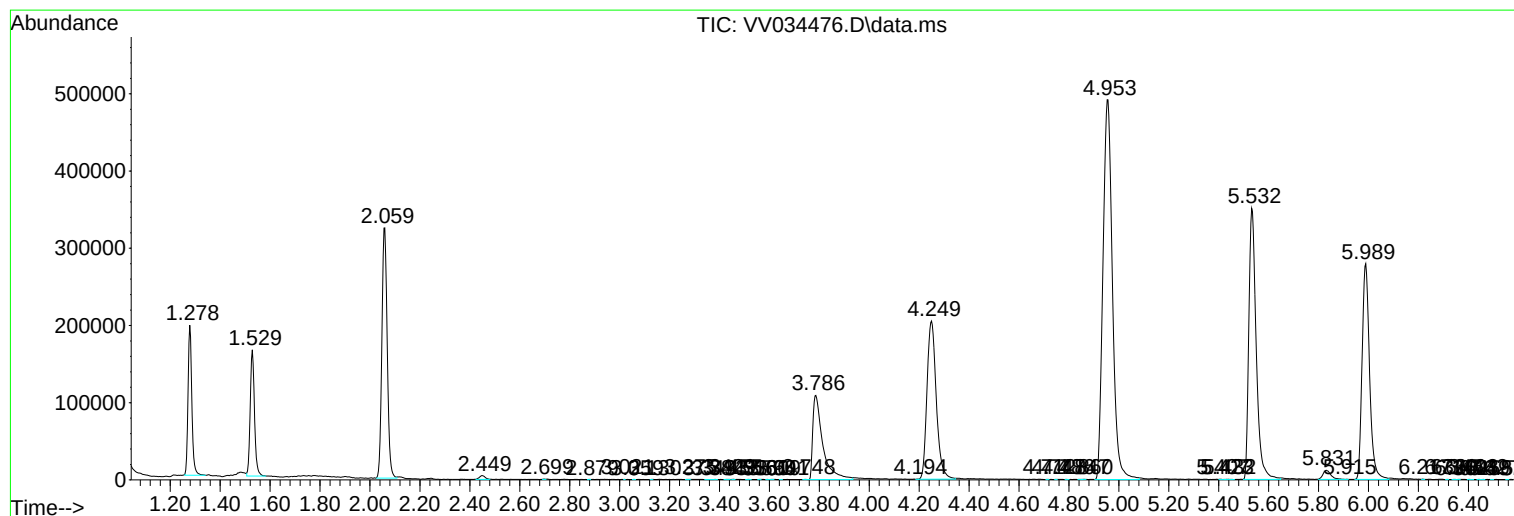

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
Data File : VV034476.D
Acq On : 29 Feb 2024 12:58
Operator : SY/MD
Sample : VV0229WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK233

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
Data File : VV034476.D
Acq On : 29 Feb 2024 12:58
Operator : SY/MD
Sample : VV0229WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK233

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------