

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
 Data File : VV034479.D
 Acq On : 29 Feb 2024 14:10
 Operator : SY/MD
 Sample : P1642-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R29

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034479.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	189717	201047	7.78%	1.604%
2	1.529	146	152	169	rVB	156676	184470	7.14%	1.471%
3	2.060	307	317	329	rBV	317703	459567	17.78%	3.666%
4	2.294	388	390	396	rVB3	465	395	0.02%	0.003%
5	2.320	396	398	399	rBV3	372	137	0.01%	0.001%
6	2.346	404	406	409	rBV	345	268	0.01%	0.002%
7	2.391	418	420	424	rVB2	413	228	0.01%	0.002%
8	2.452	432	439	448	rBV5	1490	2358	0.09%	0.019%
9	2.677	506	509	511	rBV	244	143	0.01%	0.001%
10	2.751	526	532	534	rBV2	205	243	0.01%	0.002%
11	2.838	554	559	563	rBV	440	314	0.01%	0.003%
12	2.879	569	572	575	rVB2	165	108	0.00%	0.001%
13	2.902	575	579	583	rBV2	241	259	0.01%	0.002%
14	3.076	630	633	636	rVB2	167	106	0.00%	0.001%
15	3.095	636	639	641	rBV2	213	118	0.00%	0.001%
16	3.262	688	691	692	rBV	173	103	0.00%	0.001%
17	3.330	708	712	714	rBV	175	149	0.01%	0.001%
18	3.358	718	721	724	rVB2	167	121	0.00%	0.001%
19	3.384	724	729	733	rBV2	196	236	0.01%	0.002%
20	3.432	740	744	746	rBV2	189	144	0.01%	0.001%
21	3.645	806	810	814	rBV	216	161	0.01%	0.001%
22	3.664	814	816	822	rBV2	140	151	0.01%	0.001%
23	3.738	836	839	841	rBV2	142	92	0.00%	0.001%
24	3.789	845	855	886	rBV2	121832	368052	14.24%	2.936%
25	4.249	982	998	1027	rBV	199516	512999	19.85%	4.092%
26	4.770	1157	1160	1161	rBV	179	97	0.00%	0.001%
27	4.825	1175	1177	1179	rBV	216	144	0.01%	0.001%
28	4.870	1186	1191	1198	rVB3	250	300	0.01%	0.002%
29	4.953	1198	1217	1261	rBV2	476799	1275533	49.35%	10.175%
30	5.374	1345	1348	1353	rVB3	345	270	0.01%	0.002%
31	5.397	1353	1355	1358	rVB	358	169	0.01%	0.001%
32	5.416	1358	1361	1363	rBV3	250	206	0.01%	0.002%
33	5.532	1386	1397	1430	rBV	339061	703650	27.23%	5.613%
34	5.776	1470	1473	1474	rBV	340	190	0.01%	0.002%
35	5.828	1478	1489	1515	rVB4	15714	36976	1.43%	0.295%
36	5.989	1526	1539	1566	rBV	274538	563130	21.79%	4.492%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
 Data File : VV034479.D
 Acq On : 29 Feb 2024 14:10
 Operator : SY/MD
 Sample : P1642-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R29

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.275	1626	1628	1632	rBV2	451	283	0.01%	0.002%
38	6.301	1634	1636	1640	rVB	216	117	0.00%	0.001%
39	6.397	1664	1666	1669	rBV	239	150	0.01%	0.001%
40	6.448	1677	1682	1684	rBV2	355	249	0.01%	0.002%
41	6.522	1702	1705	1710	rBV2	168	153	0.01%	0.001%
42	6.583	1721	1724	1725	rBV2	414	286	0.01%	0.002%
43	6.661	1744	1748	1751	rBV2	338	218	0.01%	0.002%
44	6.722	1765	1767	1770	rVB2	365	176	0.01%	0.001%
45	6.744	1770	1774	1778	rBV4	377	332	0.01%	0.003%
46	6.786	1785	1787	1791	rVB2	223	118	0.00%	0.001%
47	6.815	1791	1796	1797	rBV2	108	91	0.00%	0.001%
48	6.844	1801	1805	1808	rBV2	280	185	0.01%	0.001%
49	6.911	1816	1826	1853	rBV	145180	275381	10.65%	2.197%
50	7.146	1891	1899	1901	rBV4	701	922	0.04%	0.007%
51	7.243	1918	1929	1956	rBV	556939	976163	37.77%	7.787%
52	7.554	2016	2026	2055	rBV	97634	180596	6.99%	1.441%
53	7.741	2080	2084	2092	rVB3	461	584	0.02%	0.005%
54	7.773	2092	2094	2095	rBV	308	137	0.01%	0.001%
55	7.815	2104	2107	2111	rBV2	394	366	0.01%	0.003%
56	7.831	2111	2112	2114	rVB2	321	100	0.00%	0.001%
57	8.024	2162	2172	2203	rBV	384683	681906	26.38%	5.439%
58	8.577	2340	2344	2346	rVB	346	244	0.01%	0.002%
59	8.596	2346	2350	2355	rBV3	222	164	0.01%	0.001%
60	8.641	2361	2364	2365	rBV2	194	109	0.00%	0.001%
61	8.696	2379	2381	2385	rVB2	463	208	0.01%	0.002%
62	8.728	2389	2391	2393	rVB	424	118	0.00%	0.001%
63	8.783	2397	2408	2440	rBV	513376	950510	36.78%	7.582%
64	9.034	2482	2486	2487	rBV	270	161	0.01%	0.001%
65	9.062	2492	2495	2498	rBV2	221	162	0.01%	0.001%
66	9.226	2544	2546	2548	rVB2	215	104	0.00%	0.001%
67	9.304	2567	2570	2571	rBV	220	103	0.00%	0.001%
68	9.316	2571	2574	2576	rBV	160	88	0.00%	0.001%
69	9.480	2617	2625	2627	rBV2	282	297	0.01%	0.002%
70	9.545	2642	2645	2647	rBV	250	154	0.01%	0.001%
71	9.615	2664	2667	2670	rVV3	296	225	0.01%	0.002%
72	9.648	2674	2677	2678	rBV	161	97	0.00%	0.001%
73	9.657	2678	2680	2683	rVB2	281	130	0.01%	0.001%
74	9.728	2698	2702	2706	rBV2	252	205	0.01%	0.002%
75	9.754	2706	2710	2711	rBV	225	136	0.01%	0.001%
76	9.931	2761	2765	2770	rVB2	316	242	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
 Data File : VV034479.D
 Acq On : 29 Feb 2024 14:10
 Operator : SY/MD
 Sample : P1642-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R29

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.152	2822	2834	2859	rBV	360526	560747	21.70%	4.473%
78	10.323	2881	2887	2896	rBV2	3009	3754	0.15%	0.030%
79	10.432	2917	2921	2924	rBV	374	223	0.01%	0.002%
80	10.660	2990	2992	2994	rBV	185	96	0.00%	0.001%
81	10.857	3050	3053	3054	rBV	256	180	0.01%	0.001%
82	10.895	3062	3065	3070	rBV2	278	247	0.01%	0.002%
83	10.927	3072	3075	3076	rBV2	188	116	0.00%	0.001%
84	11.062	3111	3117	3120	rBV	289	329	0.01%	0.003%
85	11.120	3125	3135	3145	rVV	56047	87815	3.40%	0.700%
86	11.185	3145	3155	3184	rVB	537518	871607	33.72%	6.953%
87	11.506	3251	3255	3256	rBV2	633	454	0.02%	0.004%
88	11.574	3261	3276	3303	rVB2	1204874	2584543	100.00%	20.617%
89	11.750	3327	3331	3338	rBV5	654	694	0.03%	0.006%
90	11.905	3376	3379	3381	rBV2	198	104	0.00%	0.001%
91	12.258	3486	3489	3492	rBV	308	196	0.01%	0.002%
92	12.352	3516	3518	3522	rVB	289	166	0.01%	0.001%
93	12.522	3568	3571	3573	rBV2	268	177	0.01%	0.001%
94	12.580	3580	3589	3604	rBV3	20830	36419	1.41%	0.291%
95	13.197	3770	3781	3801	rBV	392402	603749	23.36%	4.816%
96	13.448	3852	3859	3869	rBV3	4633	7397	0.29%	0.059%
97	13.680	3920	3931	3948	rBV	214446	333624	12.91%	2.661%
98	14.098	4052	4061	4078	rBV5	5284	10395	0.40%	0.083%
99	14.435	4162	4166	4169	rBV3	676	573	0.02%	0.005%
100	15.336	4437	4446	4458	rVB3	31230	48008	1.86%	0.383%


Sum of corrected areas: 12536217

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
Data File : VV034479.D
Acq On : 29 Feb 2024 14:10
Operator : SY/MD
Sample : P1642-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

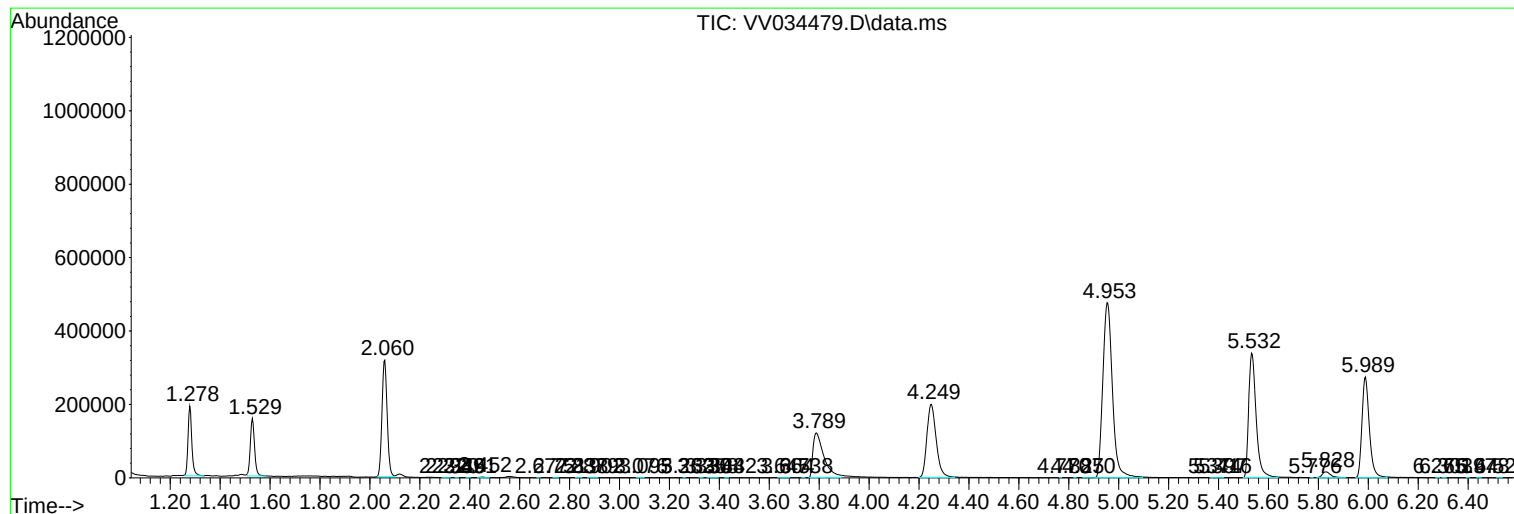

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
Data File : VV034479.D
Acq On : 29 Feb 2024 14:10
Operator : SY/MD
Sample : P1642-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
Data File : VV034479.D
Acq On : 29 Feb 2024 14:10
Operator : SY/MD
Sample : P1642-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc