

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
 Data File : VV034480.D
 Acq On : 29 Feb 2024 14:34
 Operator : SY/MD
 Sample : P1642-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034480.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	191791	202492	15.93%	2.093%
2	1.529	145	152	175	rVB	159083	192129	15.11%	1.986%
3	2.060	307	317	331	rBV	319488	462758	36.40%	4.782%
4	2.182	352	355	366	rVB5	1050	1117	0.09%	0.012%
5	2.449	433	438	444	rVB3	1396	1727	0.14%	0.018%
6	2.561	463	473	488	rBV3	4141	8326	0.65%	0.086%
7	2.661	502	504	507	rBV2	148	113	0.01%	0.001%
8	2.751	530	532	535	rBV	324	201	0.02%	0.002%
9	2.879	569	572	574	rBV2	151	92	0.01%	0.001%
10	3.085	631	636	639	rBV2	215	228	0.02%	0.002%
11	3.342	714	716	719	rVB	174	91	0.01%	0.001%
12	3.400	731	734	738	rBV2	119	93	0.01%	0.001%
13	3.474	754	757	758	rBV2	154	83	0.01%	0.001%
14	3.532	773	775	778	rBV	167	94	0.01%	0.001%
15	3.551	778	781	784	rBV	127	103	0.01%	0.001%
16	3.613	798	800	808	rBV2	165	176	0.01%	0.002%
17	3.641	808	809	813	rVB	145	67	0.01%	0.001%
18	3.664	813	816	820	rBV2	306	194	0.02%	0.002%
19	3.686	820	823	826	rBV	206	176	0.01%	0.002%
20	3.786	841	854	899	rBV2	127335	391743	30.82%	4.049%
21	4.249	983	998	1032	rBV	197746	514266	40.46%	5.315%
22	4.696	1135	1137	1138	rBV	182	73	0.01%	0.001%
23	4.786	1162	1165	1168	rBV2	350	258	0.02%	0.003%
24	4.953	1201	1217	1256	rBV2	476154	1271188	100.00%	13.137%
25	5.194	1290	1292	1294	rBV	351	134	0.01%	0.001%
26	5.268	1313	1315	1318	rBV2	275	157	0.01%	0.002%
27	5.420	1359	1362	1367	rVB	248	179	0.01%	0.002%
28	5.468	1373	1377	1379	rBV2	302	259	0.02%	0.003%
29	5.532	1386	1397	1425	rBV	350378	714597	56.21%	7.385%
30	5.828	1478	1489	1512	rBV2	21811	48823	3.84%	0.505%
31	5.905	1512	1513	1518	rVB	350	153	0.01%	0.002%
32	5.989	1526	1539	1570	rBV	274450	568166	44.70%	5.872%
33	6.198	1602	1604	1608	rVB4	549	283	0.02%	0.003%
34	6.310	1636	1639	1641	rBV	165	112	0.01%	0.001%
35	6.326	1642	1644	1646	rVB	220	76	0.01%	0.001%
36	6.371	1656	1658	1661	rVB	288	109	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
 Data File : VV034480.D
 Acq On : 29 Feb 2024 14:34
 Operator : SY/MD
 Sample : P1642-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.397	1663	1666	1668	rBV	151	108	0.01%	0.001%
38	6.468	1685	1688	1690	rBV2	154	90	0.01%	0.001%
39	6.548	1710	1713	1715	rBV	142	87	0.01%	0.001%
40	6.583	1720	1724	1726	rBV2	619	478	0.04%	0.005%
41	6.731	1766	1770	1772	rBV3	309	244	0.02%	0.003%
42	6.744	1772	1774	1775	rVV	406	190	0.01%	0.002%
43	6.767	1779	1781	1782	rBV	269	139	0.01%	0.001%
44	6.789	1786	1788	1790	rBV	195	107	0.01%	0.001%
45	6.876	1812	1815	1816	rBV2	171	84	0.01%	0.001%
46	6.911	1816	1826	1859	rVV	144863	278696	21.92%	2.880%
47	7.243	1918	1929	1953	rBV	554695	983847	77.40%	10.168%
48	7.554	2016	2026	2052	rBV	96843	181417	14.27%	1.875%
49	7.815	2106	2107	2109	rVB	239	69	0.01%	0.001%
50	7.850	2110	2118	2120	rVV3	599	620	0.05%	0.006%
51	7.870	2120	2124	2135	rVB5	2033	3617	0.28%	0.037%
52	7.931	2140	2143	2149	rBV	330	276	0.02%	0.003%
53	7.969	2153	2155	2156	rBV	187	58	0.00%	0.001%
54	8.024	2163	2172	2215	rBV	386667	695611	54.72%	7.189%
55	8.529	2328	2329	2331	rBV	314	113	0.01%	0.001%
56	8.583	2342	2346	2347	rBV	212	131	0.01%	0.001%
57	8.625	2357	2359	2363	rBV	120	76	0.01%	0.001%
58	8.644	2363	2365	2367	rVB	304	86	0.01%	0.001%
59	8.657	2367	2369	2373	rBV	197	106	0.01%	0.001%
60	8.718	2386	2388	2389	rBV	258	78	0.01%	0.001%
61	8.731	2389	2392	2394	rBV2	263	171	0.01%	0.002%
62	8.783	2397	2408	2436	rBV	511442	854074	67.19%	8.827%
63	9.091	2502	2504	2505	rBV	356	174	0.01%	0.002%
64	9.165	2524	2527	2531	rVB2	320	197	0.02%	0.002%
65	9.265	2552	2558	2559	rBV2	259	190	0.01%	0.002%
66	9.323	2574	2576	2577	rBV2	174	79	0.01%	0.001%
67	9.384	2593	2595	2597	rBV	180	79	0.01%	0.001%
68	9.397	2597	2599	2601	rVV	119	60	0.00%	0.001%
69	9.429	2605	2609	2613	rVB2	216	174	0.01%	0.002%
70	9.452	2613	2616	2618	rBV2	184	134	0.01%	0.001%
71	9.554	2647	2648	2649	rBV	241	63	0.00%	0.001%
72	9.564	2649	2651	2652	rVV	265	102	0.01%	0.001%
73	9.574	2652	2654	2658	rVV2	296	182	0.01%	0.002%
74	9.606	2662	2664	2666	rBV2	255	137	0.01%	0.001%
75	9.641	2671	2675	2679	rBV2	196	191	0.02%	0.002%
76	9.834	2732	2735	2737	rBV2	264	140	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
 Data File : VV034480.D
 Acq On : 29 Feb 2024 14:34
 Operator : SY/MD
 Sample : P1642-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.152	2822	2834	2853	rBV	349703	550057	43.27%	5.685%
78	10.323	2882	2887	2898	rVB2	3073	4465	0.35%	0.046%
79	10.593	2967	2971	2974	rBV2	217	179	0.01%	0.002%
80	10.734	3013	3015	3019	rVB	257	114	0.01%	0.001%
81	10.779	3026	3029	3034	rVB2	212	217	0.02%	0.002%
82	10.853	3050	3052	3053	rVB	219	55	0.00%	0.001%
83	10.873	3053	3058	3063	rBV2	449	511	0.04%	0.005%
84	11.091	3124	3126	3129	rVB	168	58	0.00%	0.001%
85	11.130	3131	3138	3144	rBV5	1196	1501	0.12%	0.016%
86	11.185	3144	3155	3186	rVV	517034	814677	64.09%	8.419%
87	11.345	3202	3205	3209	rBV2	401	342	0.03%	0.004%
88	11.561	3260	3272	3299	rBV	544904	892767	70.23%	9.226%
89	11.818	3347	3352	3357	rBV3	390	467	0.04%	0.005%
90	11.908	3376	3380	3383	rBV2	264	242	0.02%	0.003%
91	12.011	3410	3412	3419	rVB3	351	236	0.02%	0.002%
92	12.130	3446	3449	3451	rBV2	269	192	0.02%	0.002%
93	12.197	3461	3470	3473	rBV2	893	1228	0.10%	0.013%
94	12.422	3534	3540	3542	rBV2	271	297	0.02%	0.003%
95	12.570	3583	3586	3590	rBV2	300	229	0.02%	0.002%
96	12.670	3615	3617	3619	rBV2	266	138	0.01%	0.001%
97	13.204	3775	3783	3795	rBV4	8698	14412	1.13%	0.149%
98	13.686	3924	3933	3945	rVB4	6568	9725	0.77%	0.101%
99	13.882	3990	3994	3999	rBV2	428	447	0.04%	0.005%
100	14.455	4169	4172	4173	rBV	607	324	0.03%	0.003%




Sum of corrected areas: 9676191

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
Data File : VV034480.D
Acq On : 29 Feb 2024 14:34
Operator : SY/MD
Sample : P1642-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

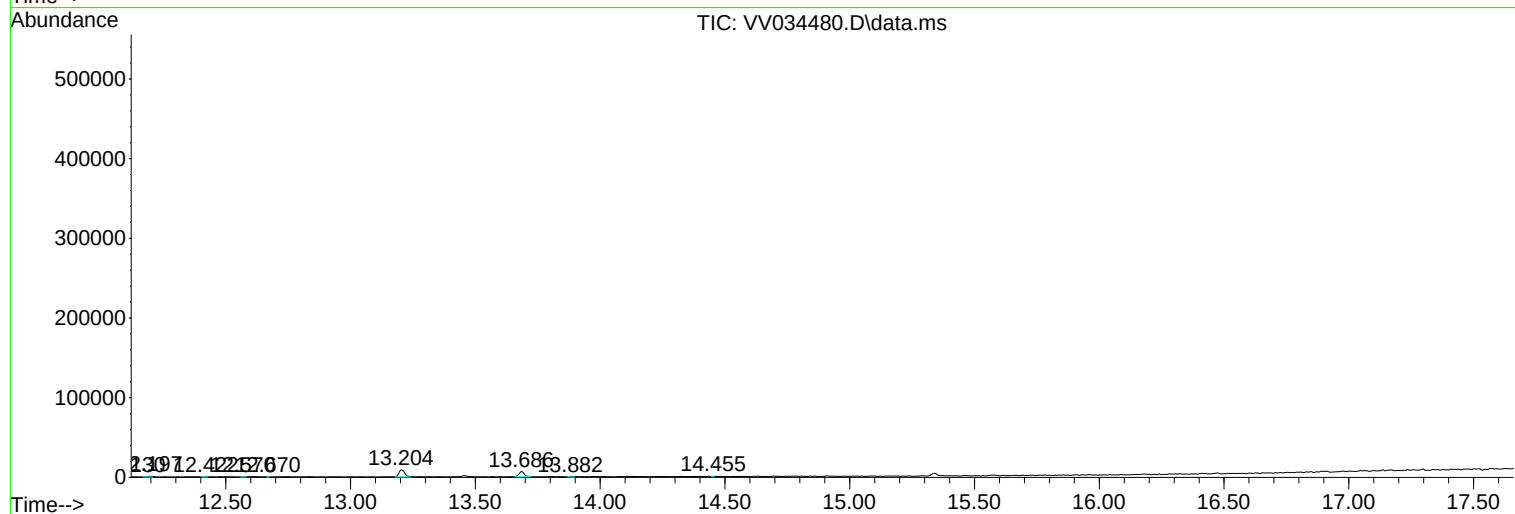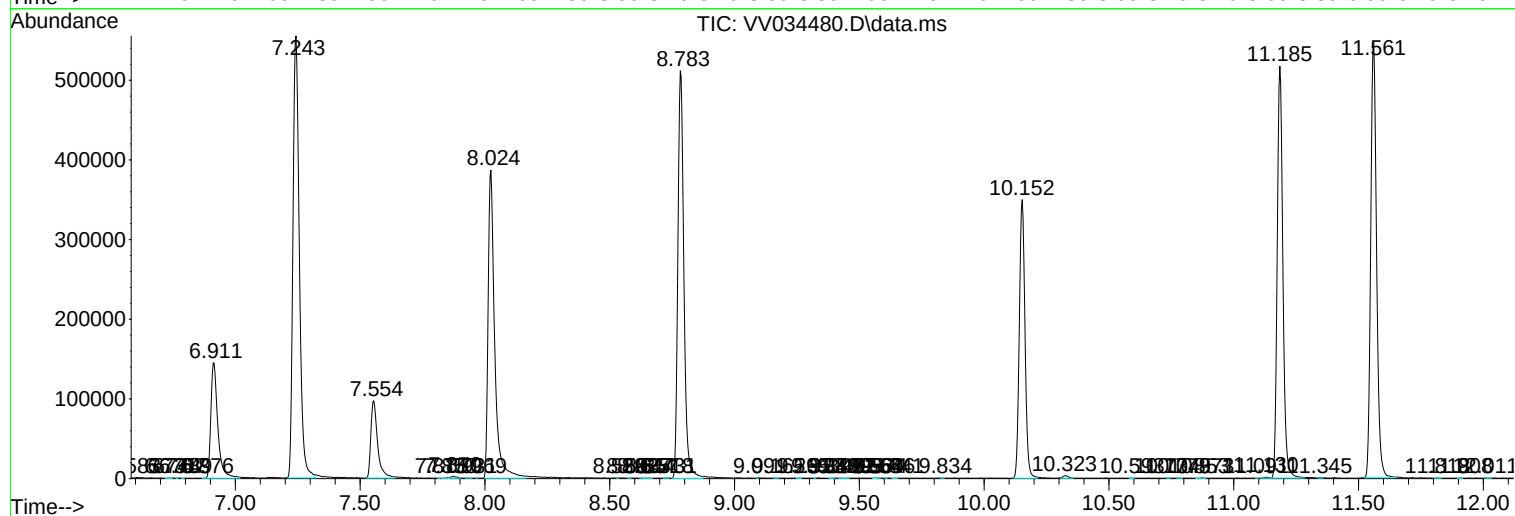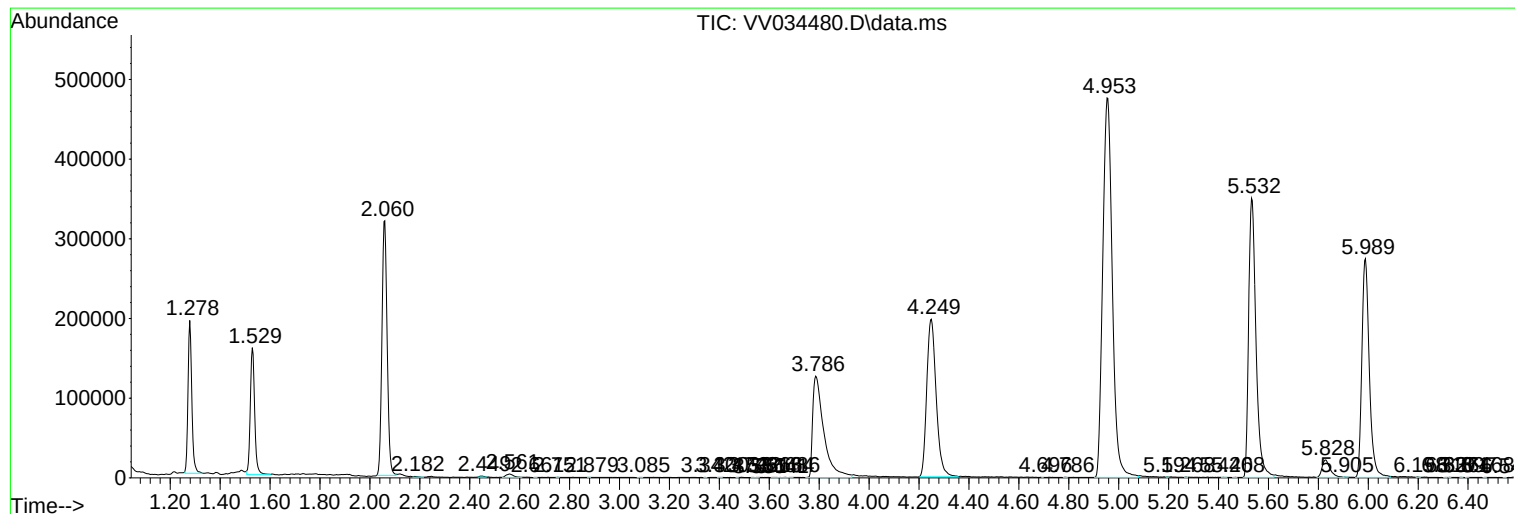

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
Data File : VV034480.D
Acq On : 29 Feb 2024 14:34
Operator : SY/MD
Sample : P1642-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
Data File : VV034480.D
Acq On : 29 Feb 2024 14:34
Operator : SY/MD
Sample : P1642-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc