

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
 Data File : VV034482.D
 Acq On : 29 Feb 2024 15:24
 Operator : SY/MD
 Sample : P1642-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M

Title : VOC Analysis

Signal : TIC: VV034482.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	179175	190024	15.59%	2.043%
2	1.529	145	152	169	rVB	150557	180137	14.78%	1.937%
3	2.059	307	317	335	rBV	301808	437921	35.94%	4.709%
4	2.281	383	386	392	rBV3	369	385	0.03%	0.004%
5	2.449	432	438	447	rVB3	1781	2863	0.23%	0.031%
6	2.677	506	509	512	rBV	275	160	0.01%	0.002%
7	2.770	535	538	541	rBV	154	151	0.01%	0.002%
8	2.944	589	592	595	rBV2	159	105	0.01%	0.001%
9	3.146	649	655	658	rBV2	219	196	0.02%	0.002%
10	3.166	658	661	664	rBV2	131	109	0.01%	0.001%
11	3.233	679	682	688	rBV2	143	116	0.01%	0.001%
12	3.352	717	719	724	rVB	229	149	0.01%	0.002%
13	3.403	732	735	738	rVB2	194	127	0.01%	0.001%
14	3.423	738	741	744	rBV	201	140	0.01%	0.002%
15	3.465	750	754	759	rVB2	116	128	0.01%	0.001%
16	3.487	759	761	764	rBV	151	103	0.01%	0.001%
17	3.506	764	767	771	rVV	169	120	0.01%	0.001%
18	3.555	778	782	784	rBV2	159	116	0.01%	0.001%
19	3.587	788	792	794	rBV	192	127	0.01%	0.001%
20	3.638	804	808	810	rBV	221	179	0.01%	0.002%
21	3.664	813	816	819	rBV	253	204	0.02%	0.002%
22	3.699	823	827	830	rBV2	185	154	0.01%	0.002%
23	3.786	845	854	896	rBV3	121131	364619	29.92%	3.921%
24	4.249	982	998	1035	rBV	195129	501465	41.15%	5.392%
25	4.622	1111	1114	1116	rBV2	315	204	0.02%	0.002%
26	4.677	1129	1131	1134	rVB	342	199	0.02%	0.002%
27	4.702	1136	1139	1142	rVV2	309	181	0.01%	0.002%
28	4.764	1155	1158	1161	rBV	294	212	0.02%	0.002%
29	4.812	1171	1173	1178	rBV2	293	211	0.02%	0.002%
30	4.841	1178	1182	1183	rBV2	274	163	0.01%	0.002%
31	4.953	1199	1217	1252	rBV2	460920	1218555	100.00%	13.103%
32	5.320	1329	1331	1338	rBV5	419	363	0.03%	0.004%
33	5.413	1354	1360	1362	rBV2	360	364	0.03%	0.004%
34	5.477	1379	1380	1383	rBV2	228	103	0.01%	0.001%
35	5.532	1386	1397	1431	rBV	351644	724526	59.46%	7.791%
36	5.831	1478	1490	1507	rBV2	20214	43438	3.56%	0.467%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
 Data File : VV034482.D
 Acq On : 29 Feb 2024 15:24
 Operator : SY/MD
 Sample : P1642-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	5.921	1516	1518	1520	rBV	346	168	0.01%	0.002%
38	5.989	1524	1539	1571	rBV	263856	551236	45.24%	5.927%
39	6.217	1607	1610	1612	rBV	182	107	0.01%	0.001%
40	6.294	1632	1634	1637	rVB2	316	161	0.01%	0.002%
41	6.320	1640	1642	1648	rVV2	231	198	0.02%	0.002%
42	6.548	1710	1713	1715	rBV	164	103	0.01%	0.001%
43	6.587	1721	1725	1727	rBV2	861	720	0.06%	0.008%
44	6.741	1768	1773	1775	rBV3	332	316	0.03%	0.003%
45	6.773	1781	1783	1786	rBV2	269	178	0.01%	0.002%
46	6.854	1806	1808	1810	rBV	207	109	0.01%	0.001%
47	6.911	1816	1826	1857	rBV	138246	263536	21.63%	2.834%
48	7.243	1918	1929	1952	rBV	526698	923789	75.81%	9.933%
49	7.554	2016	2026	2048	rBV	93723	170399	13.98%	1.832%
50	7.760	2088	2090	2091	rBV	349	115	0.01%	0.001%
51	7.812	2103	2106	2108	rVB2	226	117	0.01%	0.001%
52	7.876	2117	2126	2135	rBV4	2044	3533	0.29%	0.038%
53	7.960	2148	2152	2154	rBV2	357	202	0.02%	0.002%
54	8.024	2162	2172	2211	rBV	377109	681195	55.90%	7.325%
55	8.551	2334	2336	2338	rBV	211	112	0.01%	0.001%
56	8.632	2359	2361	2363	rVB	280	104	0.01%	0.001%
57	8.677	2372	2375	2377	rBV	241	145	0.01%	0.002%
58	8.783	2395	2408	2433	rBV	521313	852169	69.93%	9.163%
59	9.098	2502	2506	2507	rBV2	403	278	0.02%	0.003%
60	9.239	2547	2550	2556	rVB3	277	291	0.02%	0.003%
61	9.268	2556	2559	2562	rBV2	308	223	0.02%	0.002%
62	9.297	2566	2568	2571	rVB2	230	110	0.01%	0.001%
63	9.316	2572	2574	2578	rVB2	403	188	0.02%	0.002%
64	9.342	2578	2582	2587	rBV	176	137	0.01%	0.001%
65	9.455	2612	2617	2620	rBV2	170	137	0.01%	0.001%
66	9.480	2621	2625	2629	rVV2	360	310	0.03%	0.003%
67	9.506	2630	2633	2636	rVV2	240	163	0.01%	0.002%
68	9.525	2636	2639	2644	rVB2	182	123	0.01%	0.001%
69	9.619	2665	2668	2673	rVB2	172	123	0.01%	0.001%
70	9.689	2685	2690	2693	rBV2	178	173	0.01%	0.002%
71	9.722	2698	2700	2705	rVV2	221	197	0.02%	0.002%
72	9.876	2745	2748	2749	rBV	251	145	0.01%	0.002%
73	9.950	2768	2771	2774	rBV2	210	139	0.01%	0.001%
74	10.152	2823	2834	2859	rBV	337133	532160	43.67%	5.722%
75	10.239	2859	2861	2862	rBV	405	117	0.01%	0.001%
76	10.326	2876	2888	2895	rBV5	2879	4140	0.34%	0.045%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
 Data File : VV034482.D
 Acq On : 29 Feb 2024 15:24
 Operator : SY/MD
 Sample : P1642-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.487	2935	2938	2942	rVB3	381	292	0.02%	0.003%
78	10.509	2942	2945	2947	rBV	186	119	0.01%	0.001%
79	10.545	2953	2956	2961	rVB2	246	210	0.02%	0.002%
80	10.570	2961	2964	2966	rBV	169	103	0.01%	0.001%
81	10.606	2970	2975	2978	rBV2	167	153	0.01%	0.002%
82	10.976	3087	3090	3093	rBV	220	151	0.01%	0.002%
83	11.127	3134	3137	3140	rBV2	385	226	0.02%	0.002%
84	11.185	3143	3155	3181	rBV	519656	805441	66.10%	8.661%
85	11.471	3241	3244	3245	rBV	342	121	0.01%	0.001%
86	11.496	3249	3252	3254	rBV	195	130	0.01%	0.001%
87	11.561	3260	3272	3289	rBV	529446	833496	68.40%	8.962%
88	11.738	3324	3327	3330	rBV3	379	193	0.02%	0.002%
89	11.754	3330	3332	3334	rVB3	398	133	0.01%	0.001%
90	11.998	3404	3408	3411	rBV	222	129	0.01%	0.001%
91	12.017	3411	3414	3419	rBV2	242	293	0.02%	0.003%
92	12.159	3456	3458	3460	rBV	193	106	0.01%	0.001%
93	12.512	3565	3568	3571	rBV	198	178	0.01%	0.002%
94	12.815	3659	3662	3666	rBV	365	227	0.02%	0.002%
95	12.892	3681	3686	3690	rVV2	234	337	0.03%	0.004%
96	13.332	3819	3823	3824	rBV	253	173	0.01%	0.002%
97	13.551	3887	3891	3893	rBV	526	330	0.03%	0.004%
98	13.686	3931	3933	3935	rBV3	887	411	0.03%	0.004%
99	13.750	3950	3953	3959	rBV3	371	432	0.04%	0.005%
100	14.403	4151	4156	4158	rBV4	572	511	0.04%	0.005%




Sum of corrected areas: 9300078

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
Data File : VV034482.D
Acq On : 29 Feb 2024 15:24
Operator : SY/MD
Sample : P1642-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

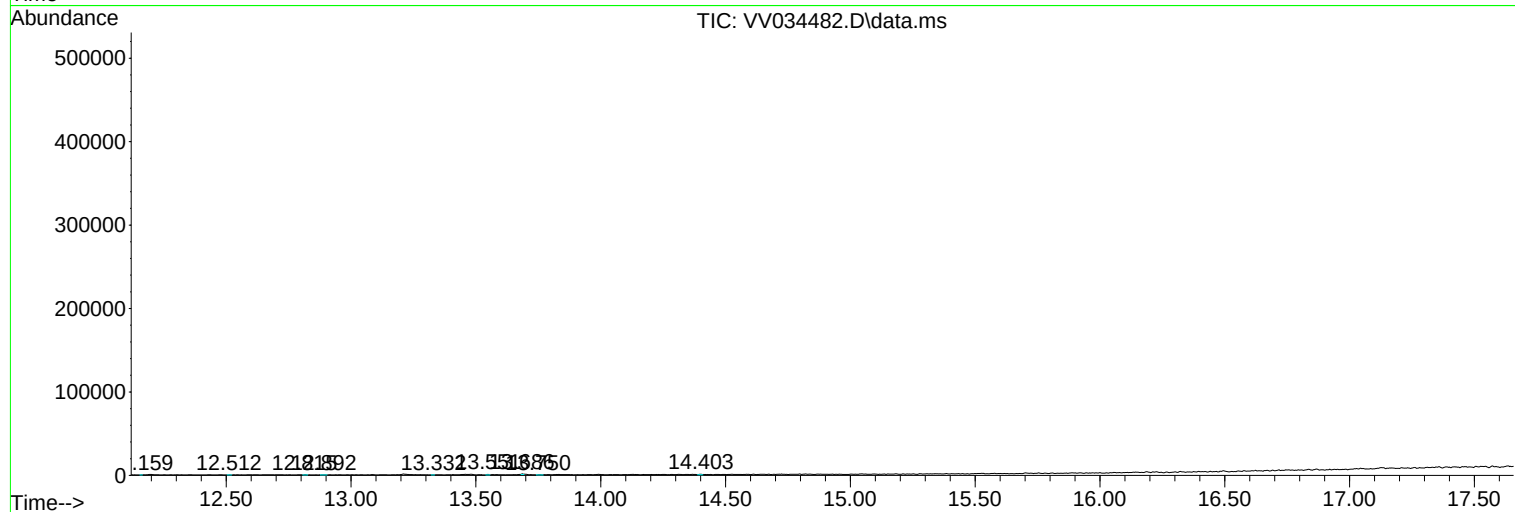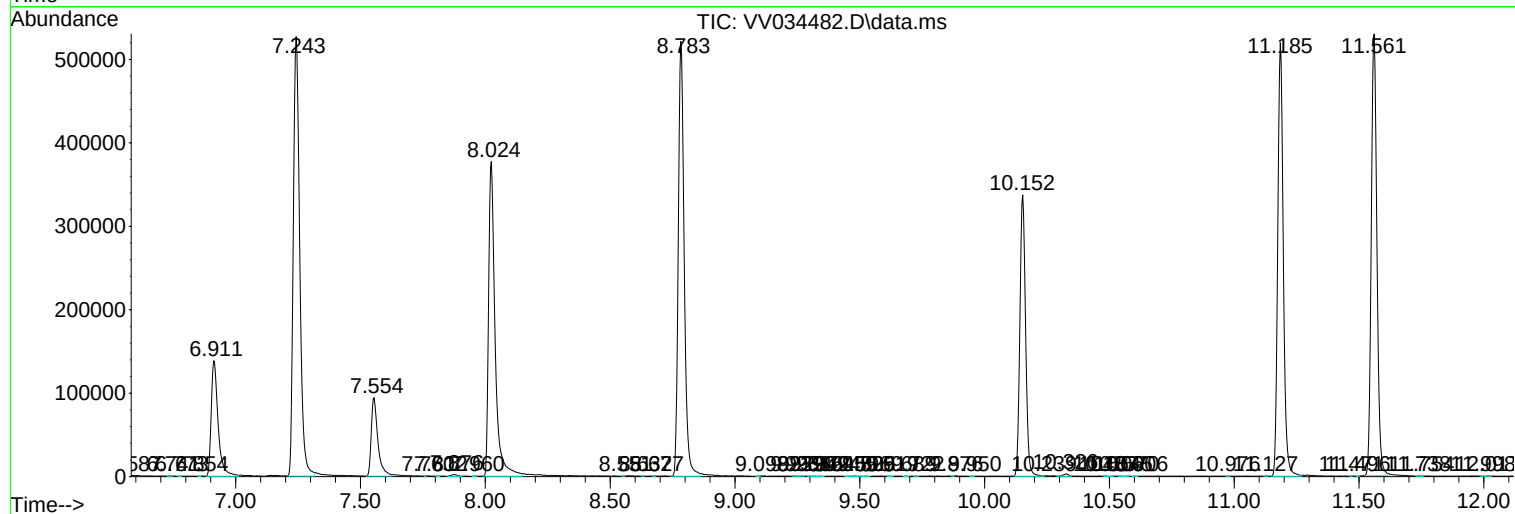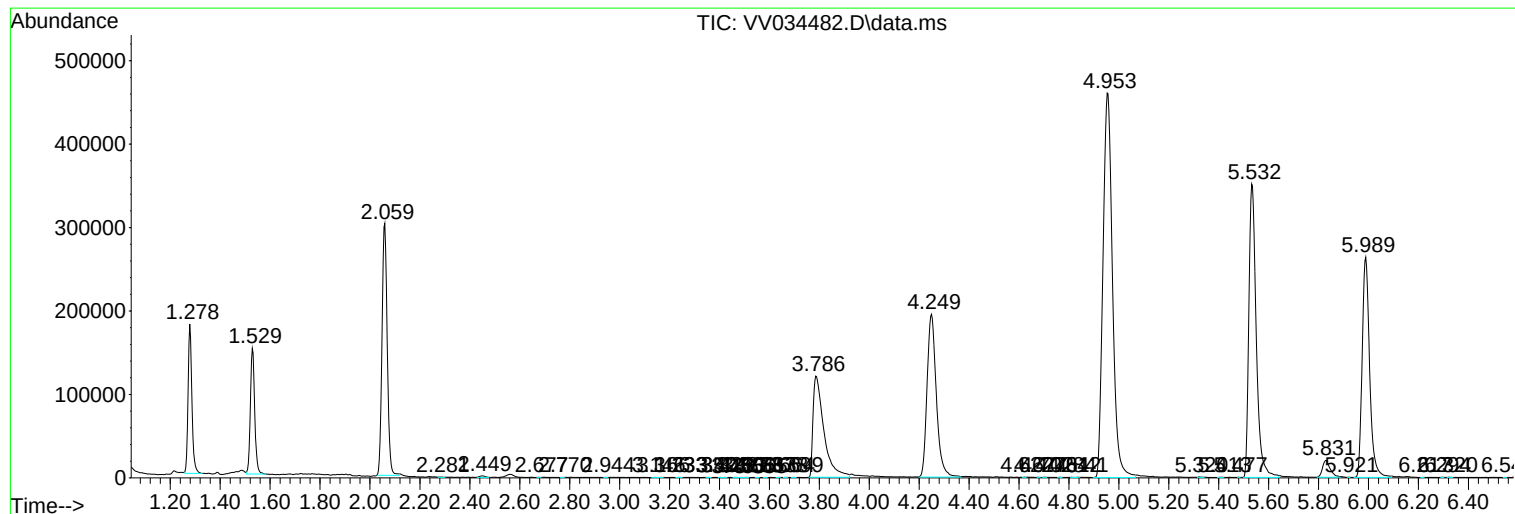

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
Data File : VV034482.D
Acq On : 29 Feb 2024 15:24
Operator : SY/MD
Sample : P1642-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
Data File : VV034482.D
Acq On : 29 Feb 2024 15:24
Operator : SY/MD
Sample : P1642-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc