


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022924\
Data File : VV034468.D
Acq On : 29 Feb 2024 08:27
Operator : SY/MD
Sample : BFB262
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB262

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Title : VOC Analysis
Last Update : Fri Mar 01 01:27:30 2024

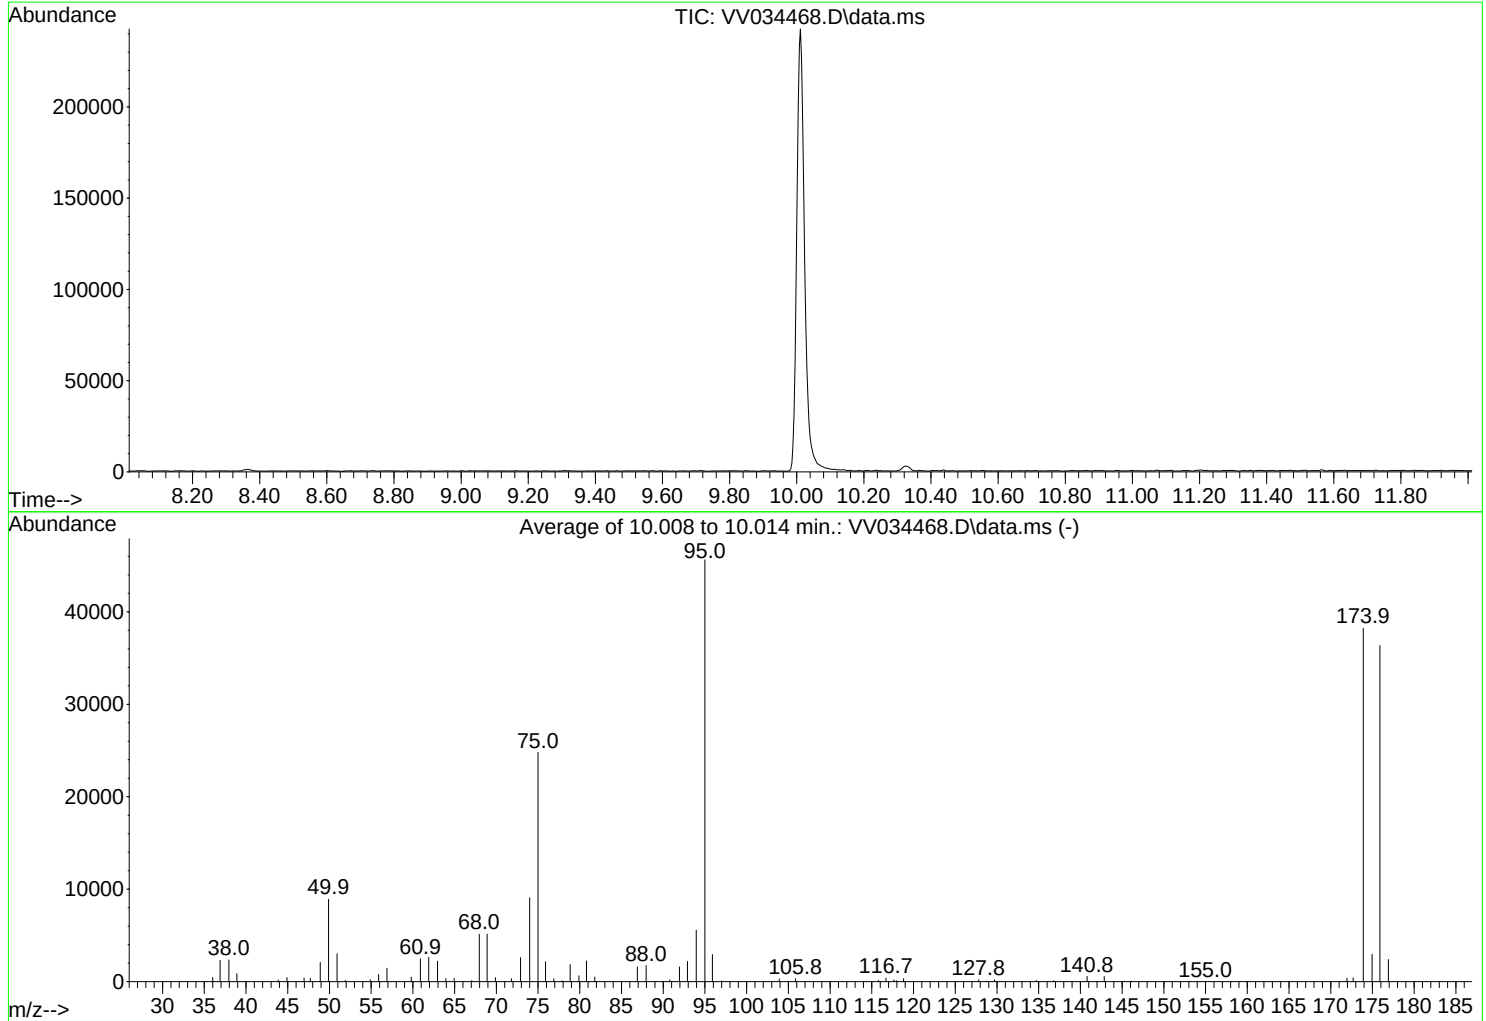

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.6	8922	PASS
75	95	30	80	54.3	24797	PASS
95	95	100	100	100.0	45627	PASS
96	95	5	9	6.4	2922	PASS
173	174	0.00	2	1.1	409	PASS
174	95	50	120	83.8	38229	PASS
175	174	5	9	7.8	2964	PASS
176	174	95	105	95.1	36360	PASS
177	176	5	10	6.6	2390	PASS

m/z	Abundance
39.90	288.0
43.90	244.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262

m/z	Abundance
36.00	455.0
36.90	2224.0
37.90	2494.0
38.90	974.0
39.90	255.0
43.80	476.0
44.90	464.0
47.00	523.0
47.70	398.0
48.90	2040.0
49.90	9058.0
50.90	3146.0
51.90	135.0
54.90	193.0
55.90	761.0
56.90	1489.0
59.80	483.0
60.90	2647.0
61.90	2430.0
63.00	2154.0
63.90	353.0
64.90	319.0
67.00	190.0
67.90	5120.0
68.90	4998.0
69.90	474.0
71.80	317.0
72.90	2794.0
74.00	9328.0
75.00	24584.0
75.90	2115.0
76.90	305.0
77.80	136.0
78.80	1732.0
79.90	652.0
80.80	2264.0
81.80	499.0
86.90	1621.0
88.00	1825.0
90.80	193.0
92.00	1739.0
92.90	2202.0
93.90	5558.0
95.00	45856.0
95.90	3056.0
97.00	126.0
103.90	311.0
105.80	325.0
115.90	140.0
116.70	372.0
117.70	183.0
118.80	300.0
127.80	215.0
129.70	169.0
134.70	122.0
136.80	102.0
140.80	593.0
142.80	519.0
172.00	412.0
172.70	407.0
173.90	37168.0
174.90	2838.0
175.90	36200.0
176.90	2363.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262

m/z	Abundance
36.00	465.0
36.90	2411.0
38.00	2432.0
38.90	890.0
39.90	282.0
43.90	414.0
44.90	468.0
46.90	386.0
47.70	352.0
48.90	2184.0
49.90	9168.0
50.90	3089.0
51.90	158.0
54.90	235.0
55.90	778.0
56.90	1502.0
59.80	498.0
60.90	2572.0
61.90	2790.0
62.90	2312.0
64.00	366.0
65.00	366.0
67.10	187.0
68.00	5338.0
68.90	5372.0
69.90	446.0
71.80	345.0
72.90	2692.0
74.00	9323.0
75.00	25560.0
75.90	2256.0
76.90	326.0
77.90	117.0
78.90	1899.0
79.90	679.0
80.80	2309.0
81.80	499.0
86.90	1650.0
88.00	1775.0
90.80	206.0
91.90	1665.0
92.90	2243.0
94.00	5779.0
95.00	47320.0
95.90	3040.0
97.00	122.0
103.90	296.0
105.90	312.0
115.70	133.0
116.70	399.0
117.60	195.0
117.90	154.0
118.80	352.0
127.80	226.0
128.70	103.0
129.70	205.0
134.70	129.0
136.80	110.0
140.80	599.0
142.80	539.0
143.90	103.0
146.10	118.0
155.00	106.0
171.90	353.0
172.70	418.0
173.90	39472.0
174.90	3067.0
175.90	37576.0
176.90	2481.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262

m/z	Abundance
36.00	431.0
36.90	2267.0
38.00	2128.0
38.90	760.0
39.90	280.0
43.90	376.0
44.90	432.0
46.90	257.0
47.70	320.0
48.90	2083.0
49.90	8539.0
50.90	2809.0
51.90	148.0
54.90	213.0
55.90	776.0
56.90	1368.0
59.80	488.0
60.90	2186.0
61.90	2659.0
62.90	2202.0
64.00	276.0
65.00	365.0
68.00	4891.0
68.90	5034.0
69.90	380.0
71.80	291.0
72.90	2315.0
74.00	8587.0
75.00	24248.0
75.90	2056.0
76.90	323.0
78.10	148.0
78.90	1918.0
79.90	611.0
80.80	2113.0
81.80	522.0
86.90	1499.0
87.90	1645.0
90.80	188.0
91.90	1392.0
92.90	2116.0
94.00	5410.0
95.00	43704.0
95.90	2670.0
103.90	258.0
105.90	280.0
115.80	136.0
116.70	369.0
117.60	182.0
118.00	168.0
118.80	337.0
127.80	192.0
128.70	102.0
129.70	178.0
134.70	126.0
136.80	125.0
140.80	518.0
142.90	606.0
146.10	116.0
171.90	332.0
172.70	403.0
173.90	38048.0
175.00	2987.0
175.90	35304.0
176.90	2327.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262