

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV030119\
 Data File : VV009447.D
 Acq On : 01 Mar 2019 11:32
 Operator : SY/MD
 Sample : K1599-20
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 02 00:22:23 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Mar 02 00:06:51 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	91671	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	85420	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	40362	5.00	ug/L	0.00

System Monitoring Compounds


4) Vinyl Chloride-d3	1.32	65	23179	4.85	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.00%
7) Chloroethane-d5	1.58	69	24697	5.71	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	114.20%
11) 1,1-Dichloroethene-d2	2.13	63	44845	3.70	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.00%
20) 2-Butanone-d5	3.96	46	50742	55.88	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.76%
24) Chloroform-d	4.40	84	49095	5.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.80%
26) 1,2-Dichloroethane-d4	5.09	65	25133	5.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.60%
32) Benzene-d6	5.10	84	101552	5.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	111.80%
36) 1,2-Dichloropropane-d6	6.12	67	30941	5.60	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	112.00%
41) Toluene-d8	7.36	98	98756	5.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.40%
43) trans-1,3-Dichloropropene-	7.67	79	12687	5.19	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	103.80%
46) 2-Hexanone-d5	8.14	63	45043	56.80	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	113.60%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	23112	5.38	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	35166	5.42	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.40%


Target Compounds					Ovalue
13) Acetone	2.21	43	5835	6.764 ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV030119\
Data File : VV009447.D
Acq On : 01 Mar 2019 11:32
Operator : SY/MD
Sample : K1599-20
Misc : 25ML/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 02 00:22:23 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Mar 02 00:06:51 2019
Response via : Initial Calibration

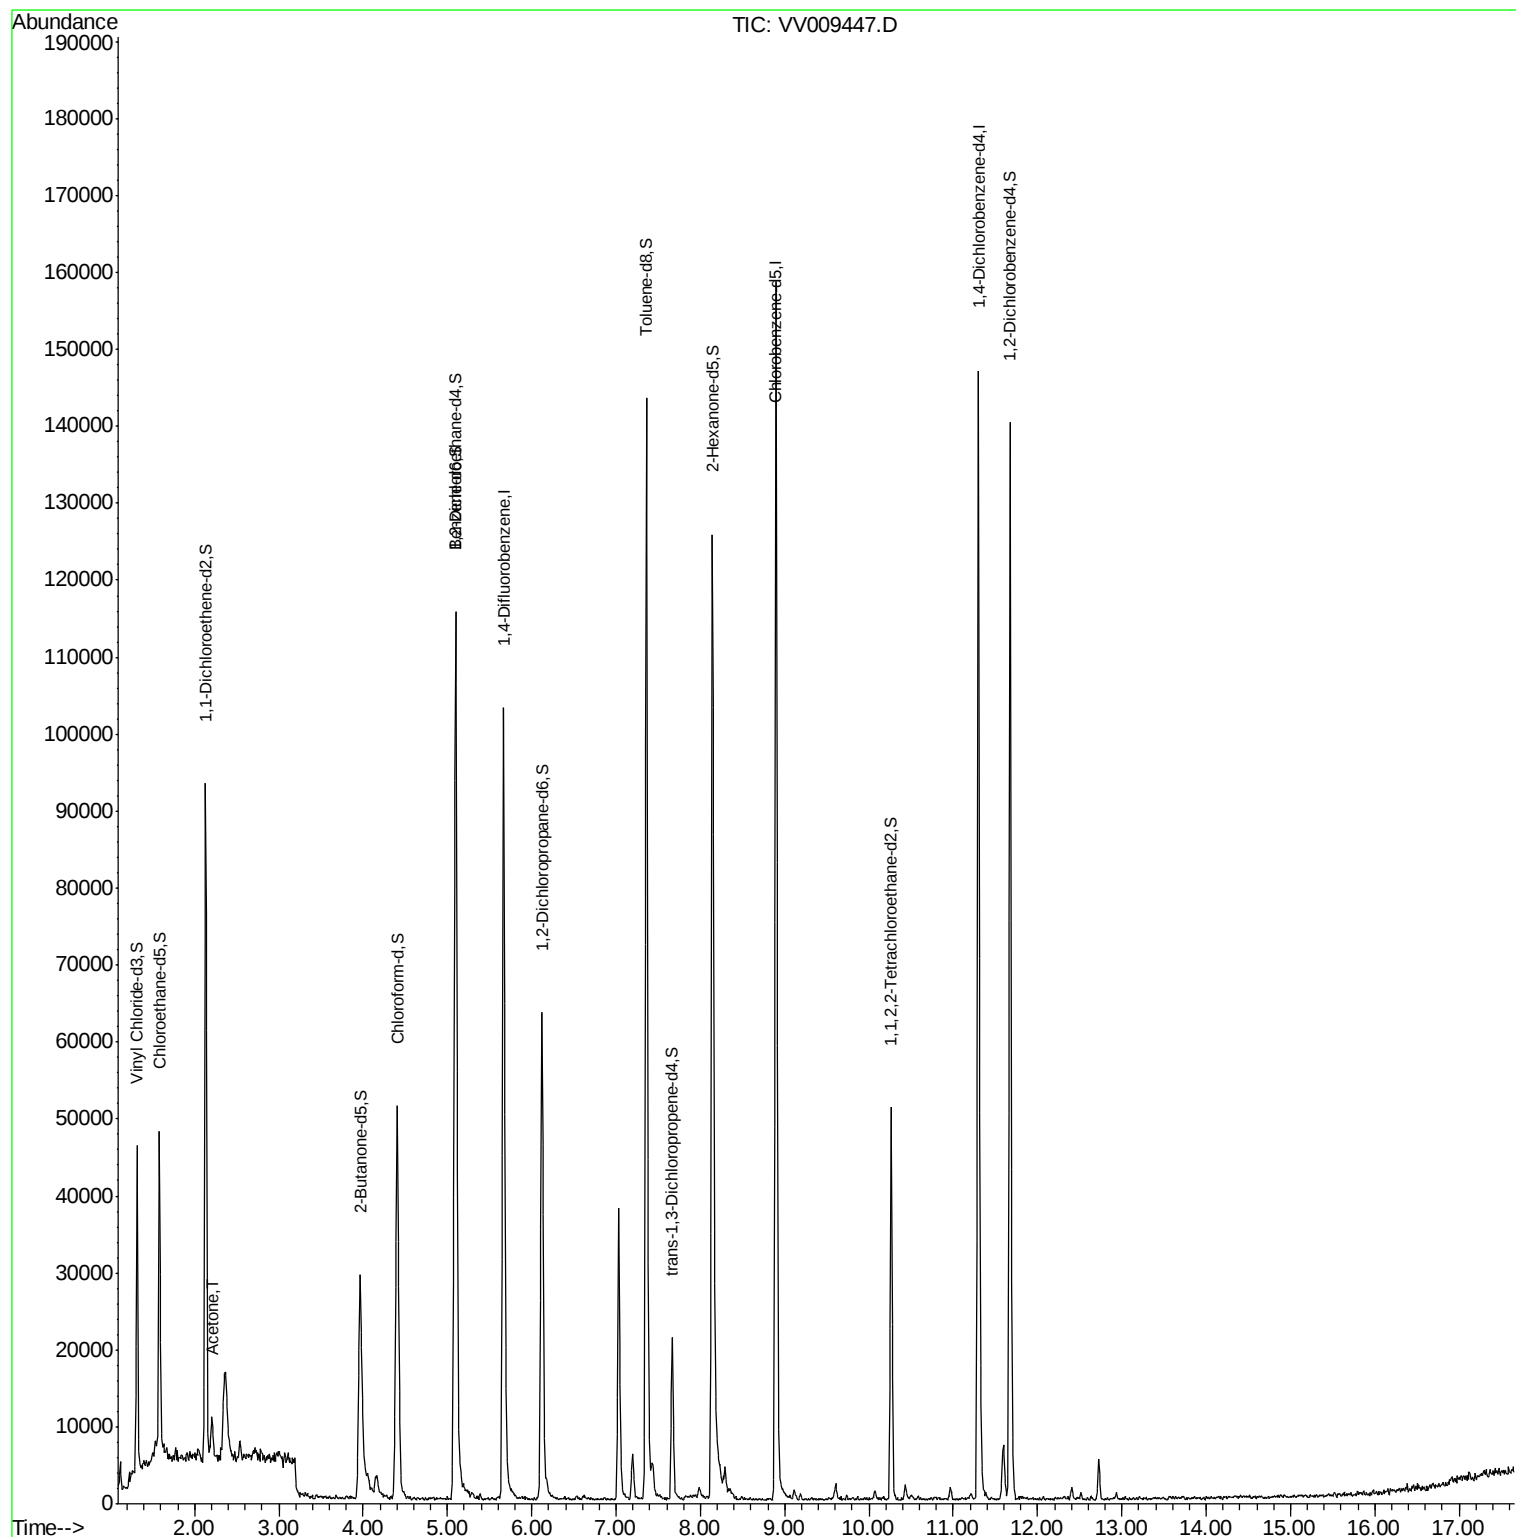

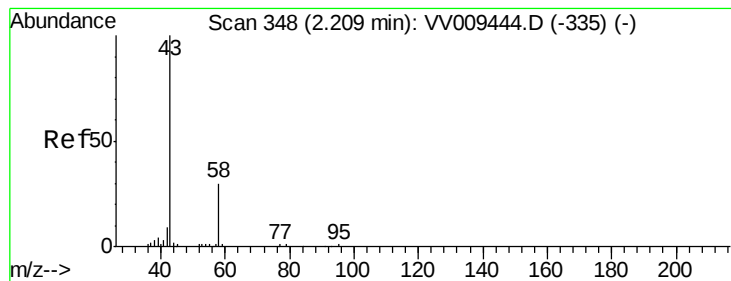

#13
 Acetone
 Concen: 6.764 ug/L
 RT: 2.21 min Scan# 347
 Delta R.T. -0.00 min
 Lab File: VV009447.D
 Acq: 01 Mar 2019 11:32

Tot Ion: 43 Resp: 5835
 Ion Ratio Lower Upper
 43 100
 58 33.1 0.0 62.0

