

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030121\
 Data File : VV020422.D
 Acq On : 01 Mar 2021 11:24
 Operator : SY/MD
 Sample : VV0301MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK168

Quant Time: Mar 02 00:15:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022621WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 02 00:15:30 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	546915	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	540270	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	268156	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	132193	48.85	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 97.70%			
7) Chloroethane-d5	1.571	69	124830	51.62	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 103.24%			
11) 1,1-Dichloroethene-d2	2.108	63	203444	36.43	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 72.86%			
21) 2-Butanone-d5	3.892	46	214511	105.28	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 105.28%			
24) Chloroform-d	4.352	84	311610	50.36	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 100.72%			
26) 1,2-Dichloroethane-d4	5.034	65	204795	52.38	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 104.76%			
32) Benzene-d6	5.053	84	624540	53.06	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 106.12%			
36) 1,2-Dichloropropane-d6	6.072	67	195123	52.96	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 105.92%			
41) Toluene-d8	7.320	98	575801	51.31	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 102.62%			
43) trans-1,3-Dichloroprop...	7.625	79	88957	50.05	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 100.10%			
47) 2-Hexanone-d5	8.092	63	136897	93.73	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 93.73%			
56) 1,1,2,2-Tetrachloroeth...	10.223	84	249277	47.71	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 95.42%			
66) 1,2-Dichlorobenzene-d4	11.632	152	265505	56.67	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 113.34%			
Target Compounds					Qvalue	
48) 2-Hexanone	8.146	43	15479	4.69	ug/L #	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030121\
Data File : VV020422.D
Acq On : 01 Mar 2021 11:24
Operator : SY/MD
Sample : VV0301MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK168

Quant Time: Mar 02 00:15:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022621WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 02 00:15:30 2021
Response via : Initial Calibration

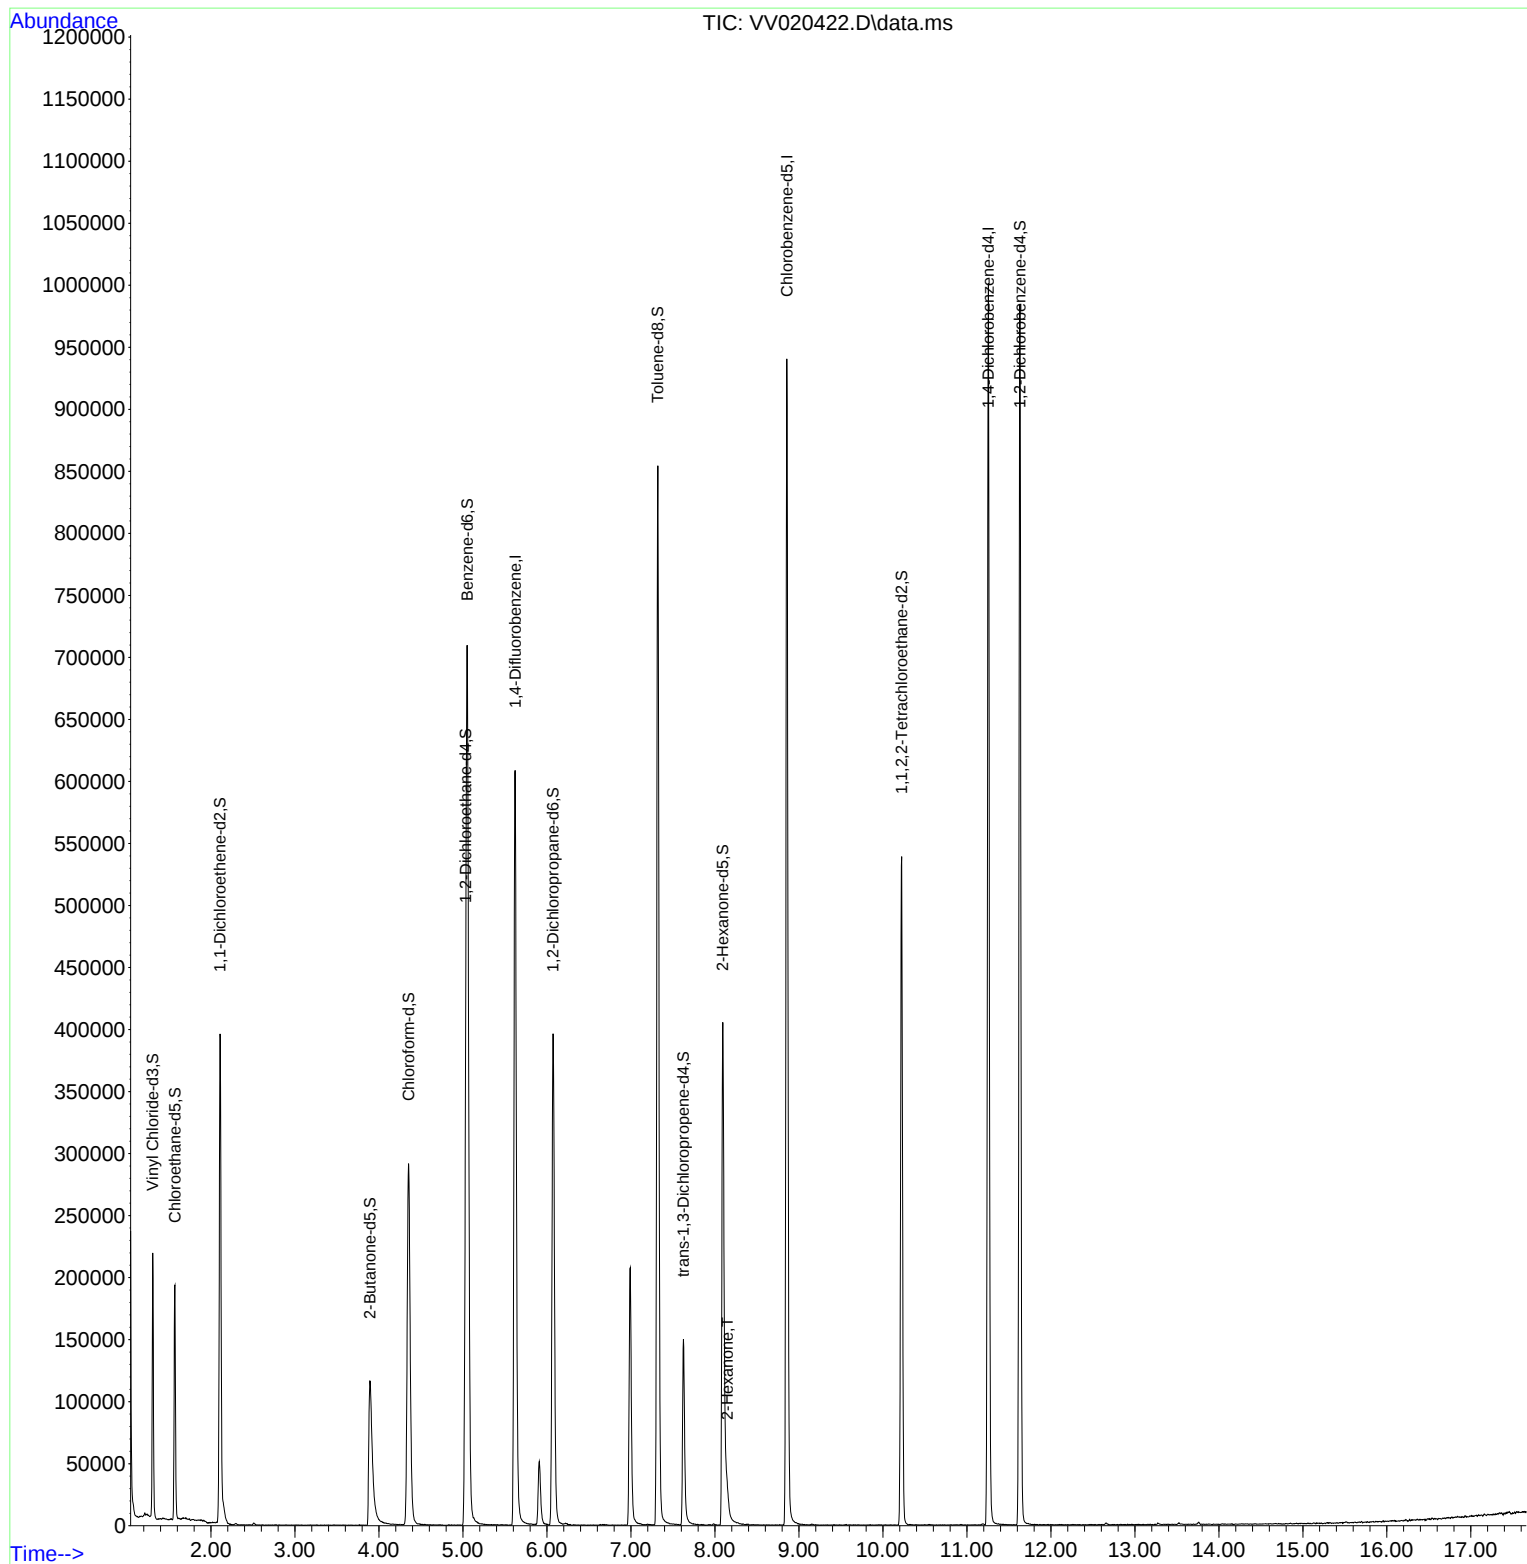

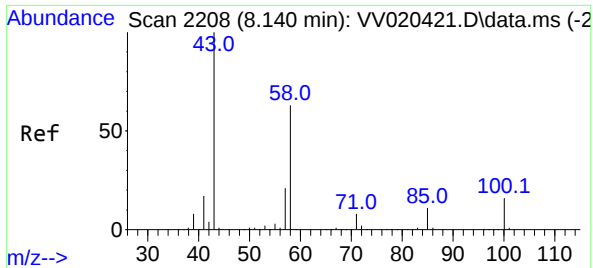

#48
2-Hexanone
Concen: 4.69 ug/L
RT: 8.146 min Scan# 2210
Delta R.T. 0.006 min
Lab File: VV020422.D
Acq: 01 Mar 2021 11:24

Instrument :
MSVOA_V
ClientSampleId :
VBLK168

Tgt Ion: 43 Resp: 15479

Ion	Ratio	Lower	Upper
43	100		
58	37.3	45.3	67.9#
57	1.6	15.8	23.6#
100	2.9	10.6	15.8#

