

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030121\
 Data File : VV020423.D
 Acq On : 01 Mar 2021 11:47
 Operator : SY/MD
 Sample : VV0301WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK169

Quant Time: Mar 02 00:16:18 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022621WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 02 00:15:30 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	556099	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	547511	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	275981	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	128034	46.53	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	93.06%
7) Chloroethane-d5	1.568	69	120646	49.06	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	98.12%
11) 1,1-Dichloroethene-d2	2.108	63	199627	35.16	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.32%
21) 2-Butanone-d5	3.886	46	210989	101.84	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	101.84%
24) Chloroform-d	4.352	84	303791	48.29	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.58%
26) 1,2-Dichloroethane-d4	5.037	65	201943	50.80	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.60%
32) Benzene-d6	5.053	84	613621	51.45	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.90%
36) 1,2-Dichloropropane-d6	6.075	67	192468	51.55	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	103.10%
41) Toluene-d8	7.320	98	562990	49.51	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.02%
43) trans-1,3-Dichloroprop...	7.625	79	85425	47.43	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.86%
47) 2-Hexanone-d5	8.091	63	138356	93.48	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.48%
56) 1,1,2,2-Tetrachloroeth...	10.223	84	247959	46.83	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	93.66%
66) 1,2-Dichlorobenzene-d4	11.631	152	260116	53.95	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.90%
Target Compounds						
48) 2-Hexanone	8.149	43	12175	3.64	ug/L	Qvalue # 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030121\
Data File : VV020423.D
Acq On : 01 Mar 2021 11:47
Operator : SY/MD
Sample : VV0301WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK169

Quant Time: Mar 02 00:16:18 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022621WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 02 00:15:30 2021
Response via : Initial Calibration

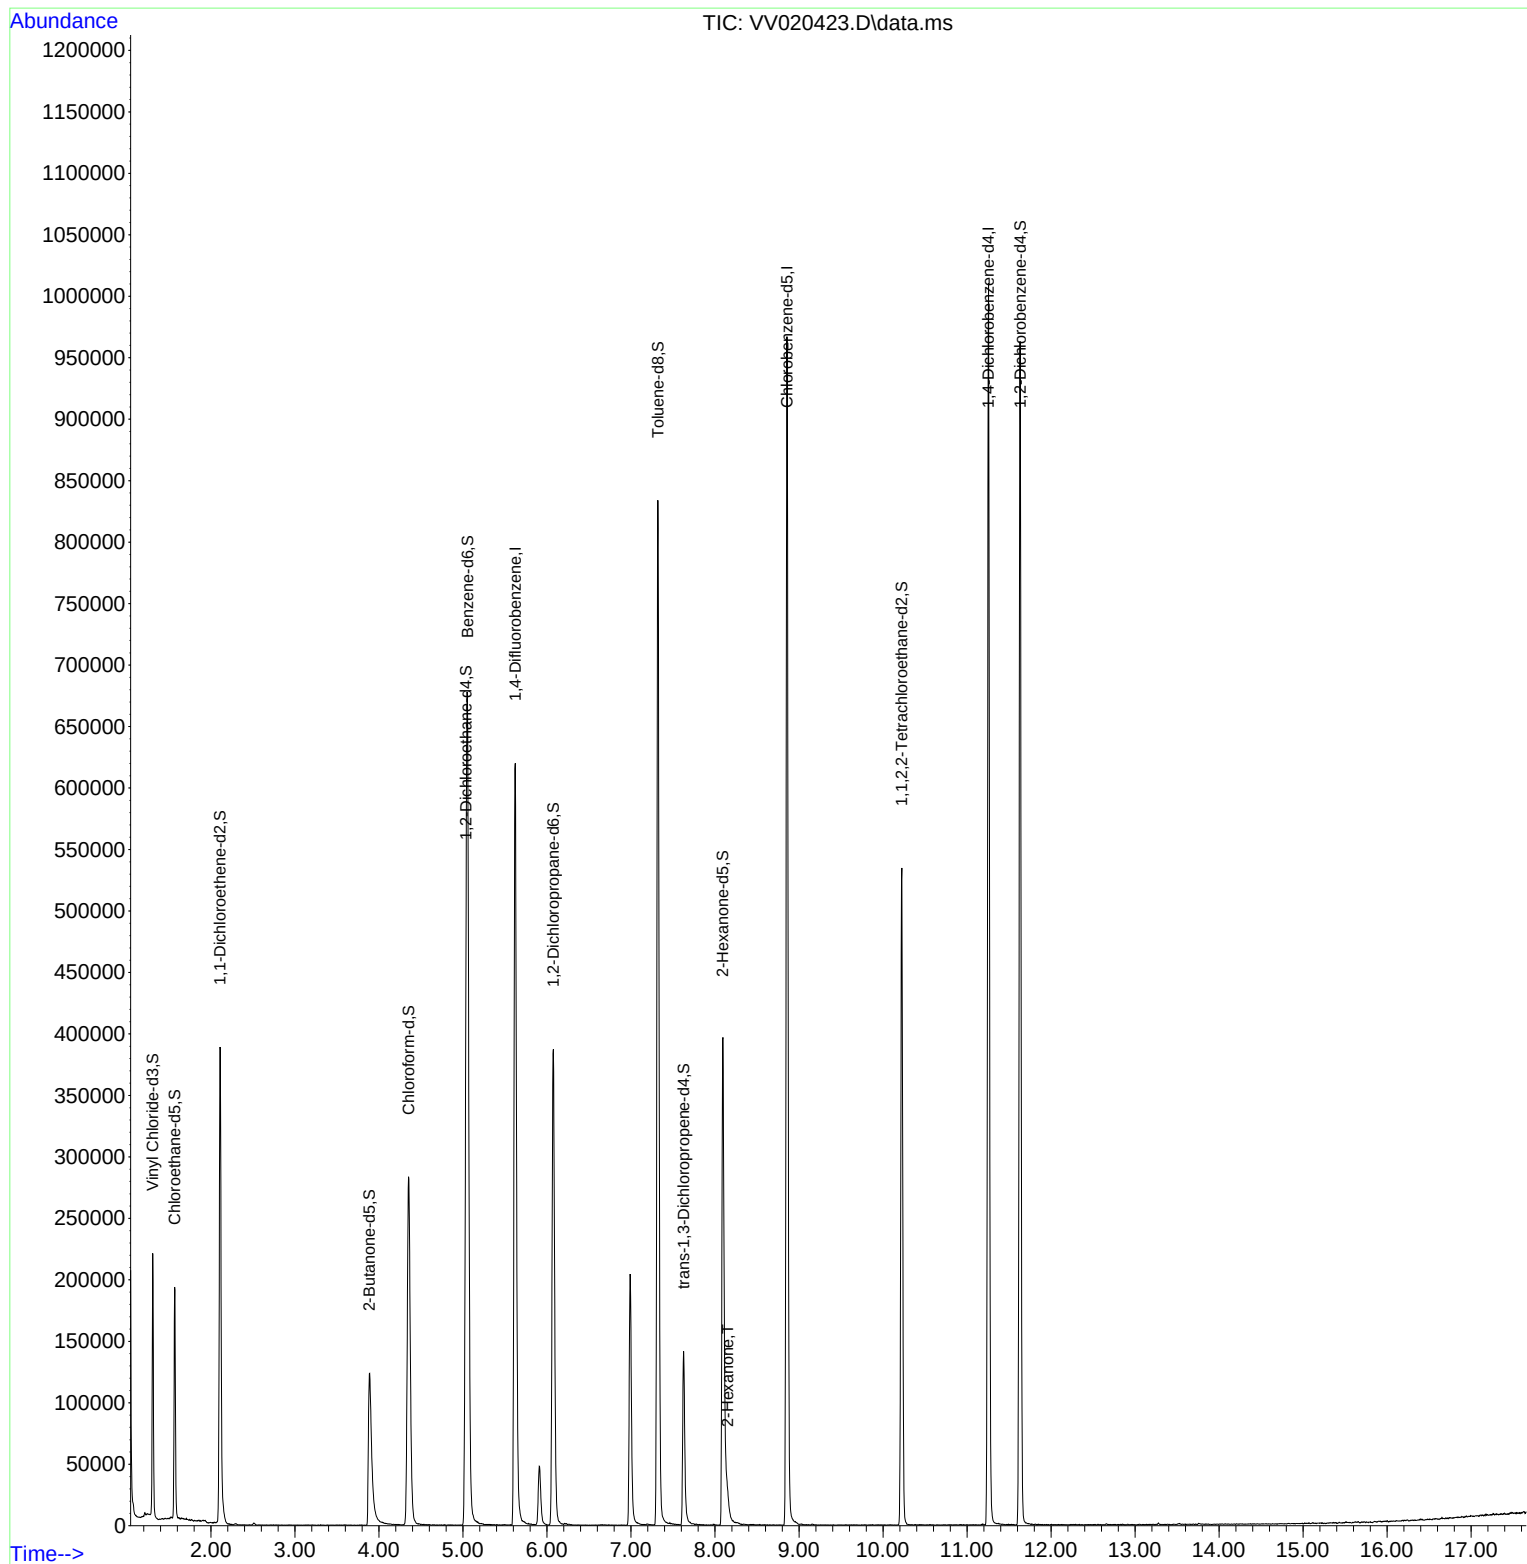

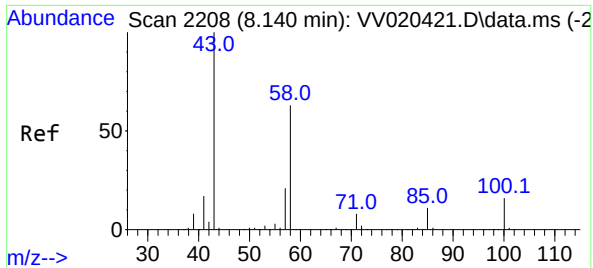

#48
2-Hexanone
Concen: 3.64 ug/L
RT: 8.149 min Scan# 2211
Delta R.T. 0.010 min
Lab File: VV020423.D
Acq: 01 Mar 2021 11:47

Instrument :
MSVOA_V
ClientSampleId :
VBLK169

Tgt Ion: 43 Resp: 12175

Ion	Ratio	Lower	Upper
43	100		
58	45.0	45.3	67.9#
57	20.0	15.8	23.6
100	9.0	10.6	15.8#

