
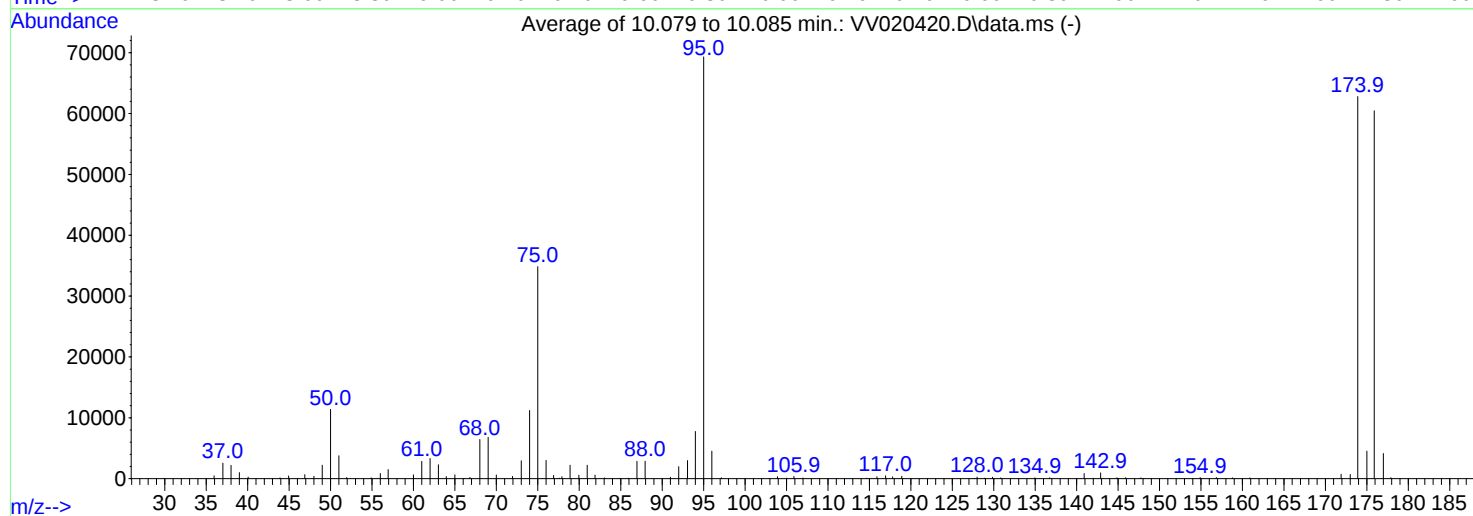


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030121\
Data File : VV020420.D
Acq On : 01 Mar 2021 09:31
Operator : SY/MD
Sample : BFB87
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB87

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022621WMA.M
Title : VOC Analysis
Last Update : Tue Mar 02 00:15:30 2021

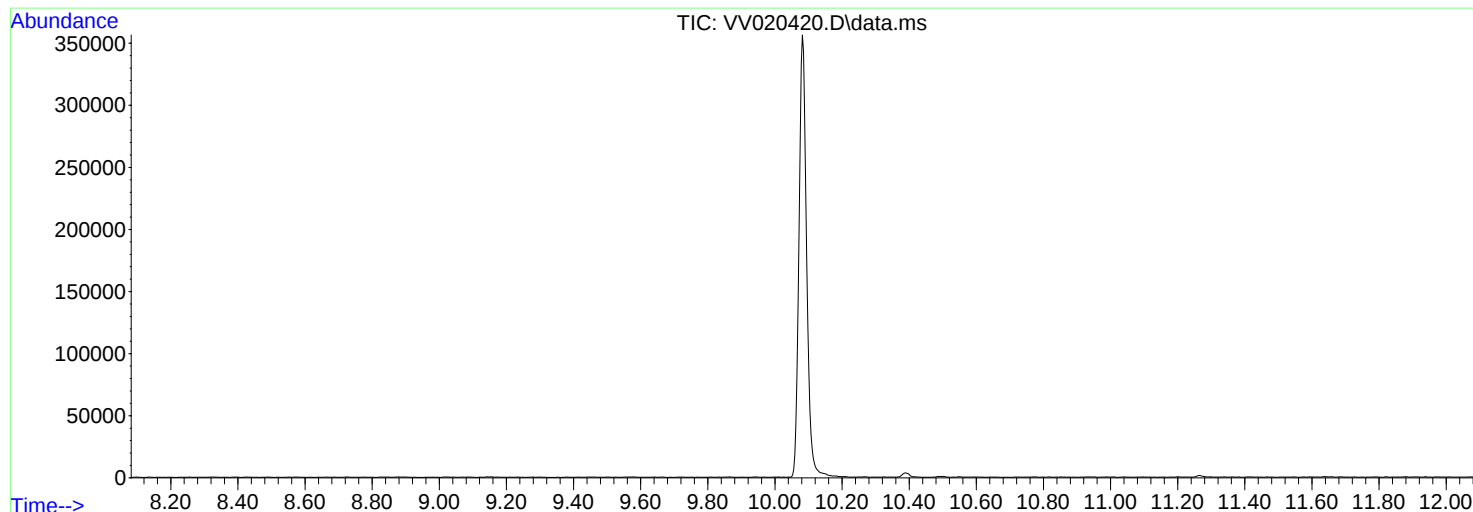

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2800

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.4	11376	PASS
75	95	30	80	50.3	34843	PASS
95	95	100	100	100.0	69325	PASS
96	95	5	9	6.5	4512	PASS
173	174	0.00	2	1.1	679	PASS
174	95	50	120	90.6	62803	PASS
175	174	5	9	7.2	4522	PASS
176	174	95	101	96.3	60469	PASS
177	176	5	9	6.8	4128	PASS

m/z	Abundance
39.80	198.0
43.80	433.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87

m/z	Abundance
36.00	404.0
37.00	2500.0
38.00	2107.0
39.00	989.0
40.00	252.0
43.90	593.0
44.90	376.0
46.90	626.0
48.00	427.0
49.00	2139.0
50.00	11085.0
51.00	3575.0
51.90	200.0
54.90	133.0
56.00	797.0
57.00	1434.0
60.00	626.0
61.00	2711.0
62.00	3344.0
63.00	2295.0
64.00	366.0
65.00	780.0
66.10	113.0
66.80	210.0
68.00	6392.0
69.00	6784.0
70.00	544.0
71.90	390.0
73.00	2887.0
74.00	11059.0
75.00	34208.0
76.00	2859.0
76.90	413.0
77.80	293.0
78.90	2200.0
80.00	600.0
80.90	2183.0
81.90	548.0
83.10	115.0
86.90	2987.0
87.90	2814.0
91.00	253.0
92.00	1915.0
93.10	3017.0
94.00	7553.0
95.00	68520.0
96.00	4519.0
97.00	144.0
103.90	287.0
105.00	119.0
105.90	365.0
114.70	118.0
115.90	312.0
116.90	495.0
117.80	262.0
118.90	394.0
127.90	275.0
129.80	244.0
130.90	151.0
134.90	110.0
136.80	144.0
140.90	856.0
141.90	104.0
142.90	944.0
144.80	152.0
145.90	151.0
147.80	146.0
150.00	100.0
154.90	186.0
156.90	166.0
158.80	127.0
160.90	149.0
171.90	808.0
173.00	713.0
173.90	63400.0
175.00	4590.0
175.90	61912.0
177.00	4069.0
177.90	175.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87

m/z	Abundance
35.90	505.0
37.00	2675.0
38.00	2272.0
39.00	1026.0
40.10	256.0
44.00	568.0
45.00	466.0
46.90	697.0
48.00	412.0
49.00	2292.0
50.00	11711.0
51.00	3882.0
51.90	212.0
54.90	137.0
56.00	878.0
57.00	1511.0
60.00	647.0
61.00	2937.0
62.00	3428.0
63.00	2331.0
64.00	349.0
65.00	650.0
66.80	243.0
68.00	6699.0
69.00	7067.0
70.00	621.0
71.90	392.0
73.00	3030.0
74.00	11606.0
75.00	36024.0
76.00	3138.0
76.90	570.0
77.90	303.0
78.90	2335.0
79.90	598.0
80.90	2288.0
81.90	599.0
83.00	132.0
85.90	118.0
87.00	2896.0
87.90	2995.0
91.00	242.0
92.00	2054.0
93.00	3066.0
94.00	8084.0
95.00	71744.0
96.00	4695.0
97.20	173.0
103.90	314.0
105.00	122.0
105.90	367.0
107.00	148.0
114.70	109.0
115.90	328.0
117.00	467.0
117.80	301.0
118.90	383.0
128.00	278.0
128.90	107.0
129.80	226.0
130.90	143.0
135.00	141.0
136.70	163.0
140.90	863.0
142.90	977.0
144.80	147.0
145.90	180.0
147.70	155.0
148.10	129.0
154.90	207.0
156.80	178.0
158.80	130.0
160.90	154.0
171.90	755.0
173.00	674.0
173.90	65256.0
175.00	4694.0
175.90	62408.0
177.00	4358.0
177.90	183.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87

m/z	Abundance
35.90	504.0
37.00	2452.0
38.00	2215.0
39.00	1000.0
40.10	250.0
44.10	537.0
45.00	502.0
46.90	651.0
48.00	334.0
49.00	2190.0
50.00	11331.0
51.00	3817.0
52.00	168.0
54.90	125.0
56.00	831.0
56.90	1536.0
60.00	594.0
61.00	2900.0
62.00	3204.0
63.00	2201.0
63.90	318.0
65.00	487.0
66.80	202.0
68.00	6217.0
69.00	6494.0
70.00	626.0
72.00	361.0
73.00	2906.0
74.00	10963.0
75.00	34296.0
76.00	2997.0
76.90	585.0
77.60	285.0
78.00	319.0
78.90	2128.0
79.90	559.0
81.00	2169.0
81.90	608.0
83.00	122.0
85.90	121.0
87.00	2616.0
88.00	2784.0
91.00	210.0
92.00	1993.0
93.00	2815.0
94.00	7666.0
95.00	67712.0
96.00	4322.0
97.20	187.0
103.90	330.0
105.90	335.0
107.00	154.0
115.90	308.0
117.00	457.0
117.80	288.0
118.90	437.0
127.70	195.0
128.10	218.0
128.90	103.0
129.90	222.0
130.80	126.0
135.00	152.0
136.70	156.0
140.90	786.0
142.10	146.0
142.90	913.0
145.00	164.0
145.90	177.0
147.80	141.0
148.90	112.0
154.90	160.0
156.80	179.0
158.80	111.0
160.90	106.0
171.90	638.0
173.00	651.0
173.90	59752.0
175.00	4282.0
175.90	57088.0
177.00	3957.0
177.90	155.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87