

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030123\
 Data File : VV030103.D
 Acq On : 01 Mar 2023 12:24
 Operator : SY/MD
 Sample : VV0301WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK305

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030103.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	87	rVB	72876	77337	15.07%	1.809%
2	1.535	147	154	170	rVB	71437	87531	17.05%	2.048%
3	2.066	307	319	337	rBV	141487	207662	40.46%	4.858%
4	2.455	432	440	454	rVB5	4048	7368	1.44%	0.172%
5	3.847	857	873	922	rBV2	30591	162568	31.67%	3.803%
6	4.265	984	1003	1033	rBV2	91174	234414	45.67%	5.484%
7	4.973	1206	1223	1256	rBV2	202138	513294	100.00%	12.008%
8	5.545	1387	1401	1427	rBV	166789	344609	67.14%	8.062%
9	6.001	1530	1543	1563	rBV	119868	245889	47.90%	5.752%
10	6.924	1816	1830	1849	rBV2	49546	94030	18.32%	2.200%
11	7.252	1920	1932	1968	rBV	235479	424775	82.75%	9.937%
12	7.564	2019	2029	2059	rBV	29682	55447	10.80%	1.297%
13	8.040	2164	2177	2212	rBV	217087	434015	84.55%	10.153%
14	8.371	2271	2280	2293	rVB3	4270	7471	1.46%	0.175%
15	8.792	2400	2411	2443	rBV	249294	416530	81.15%	9.744%
16	10.162	2823	2837	2858	rBV	93593	147774	28.79%	3.457%
17	11.194	3146	3158	3177	rBV	265203	417217	81.28%	9.760%
18	11.570	3263	3275	3292	rBV	246759	385602	75.12%	9.021%
19	12.204	3462	3472	3485	rBV2	3729	5591	1.09%	0.131%
20	13.995	4019	4029	4041	rBV2	3173	5596	1.09%	0.131%




Sum of corrected areas: 4274720

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030123\
Data File : VV030103.D
Acq On : 01 Mar 2023 12:24
Operator : SY/MD
Sample : VV0301WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK305

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

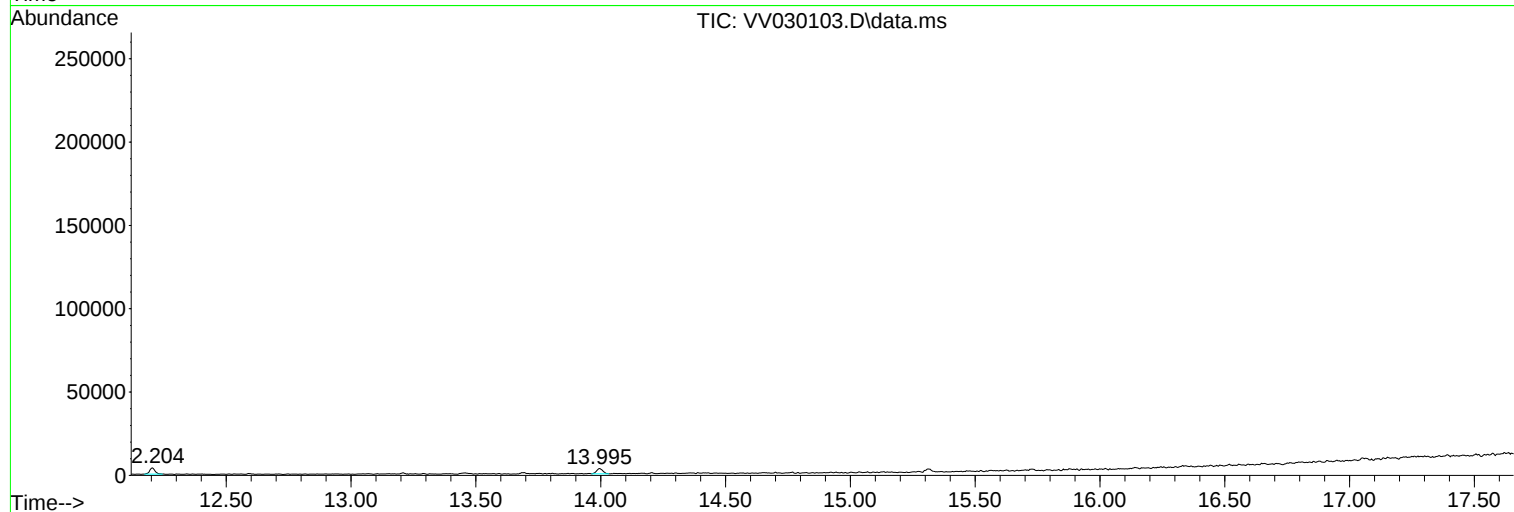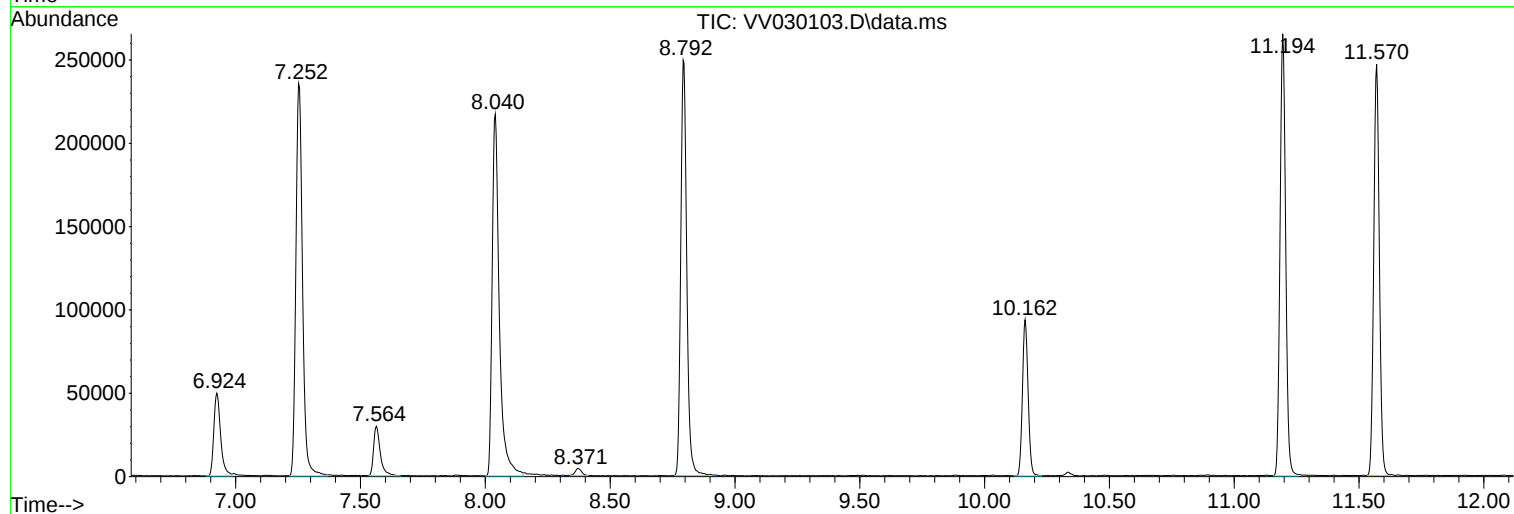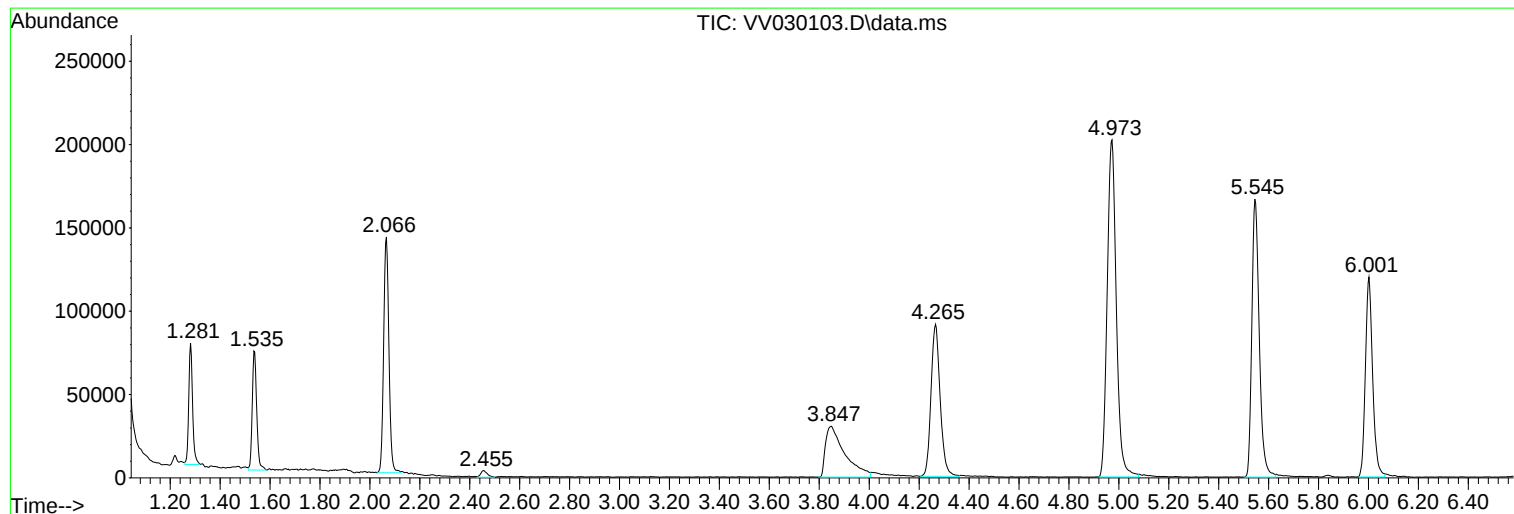

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030123\
Data File : VV030103.D
Acq On : 01 Mar 2023 12:24
Operator : SY/MD
Sample : VV0301WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK305

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030123\
Data File : VV030103.D
Acq On : 01 Mar 2023 12:24
Operator : SY/MD
Sample : VV0301WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK305

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc