

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030123\
 Data File : VV030106.D
 Acq On : 01 Mar 2023 13:40
 Operator : SY/MD
 Sample : 01729-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BZ1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030106.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	51	55	62	rBV2	5218	5618	1.09%	0.130%
2	1.281	69	75	94	rVB	72667	84487	16.44%	1.958%
3	1.539	148	155	165	rVB	72364	86675	16.87%	2.008%
4	2.066	309	319	337	rVB	139468	201143	39.14%	4.660%
5	3.825	853	866	911	rBV	42137	166835	32.47%	3.865%
6	4.262	985	1002	1032	rBV	91529	232930	45.33%	5.397%
7	4.969	1205	1222	1257	rBV2	202227	513891	100.00%	11.907%
8	5.545	1388	1401	1426	rBV	169821	347629	67.65%	8.054%
9	5.998	1526	1542	1566	rBV	119031	250341	48.71%	5.800%
10	6.924	1816	1830	1847	rBV	49186	91279	17.76%	2.115%
11	7.252	1919	1932	1967	rBV	239224	425710	82.84%	9.864%
12	7.564	2019	2029	2052	rBV2	28714	52909	10.30%	1.226%
13	7.889	2117	2130	2142	rBV2	6861	13398	2.61%	0.310%
14	8.037	2165	2176	2214	rBV	231409	427164	83.12%	9.897%
15	8.792	2399	2411	2437	rBV	256938	425217	82.74%	9.852%
16	10.162	2826	2837	2856	rVB	93962	146548	28.52%	3.395%
17	10.336	2880	2891	2902	rBV	16811	27612	5.37%	0.640%
18	11.194	3146	3158	3183	rBV	274760	424195	82.55%	9.828%
19	11.570	3263	3275	3292	rVV	243101	384149	74.75%	8.901%
20	12.204	3461	3472	3483	rVB2	5275	8280	1.61%	0.192%




Sum of corrected areas: 4316010

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030123\
Data File : VV030106.D
Acq On : 01 Mar 2023 13:40
Operator : SY/MD
Sample : 01729-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BZ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

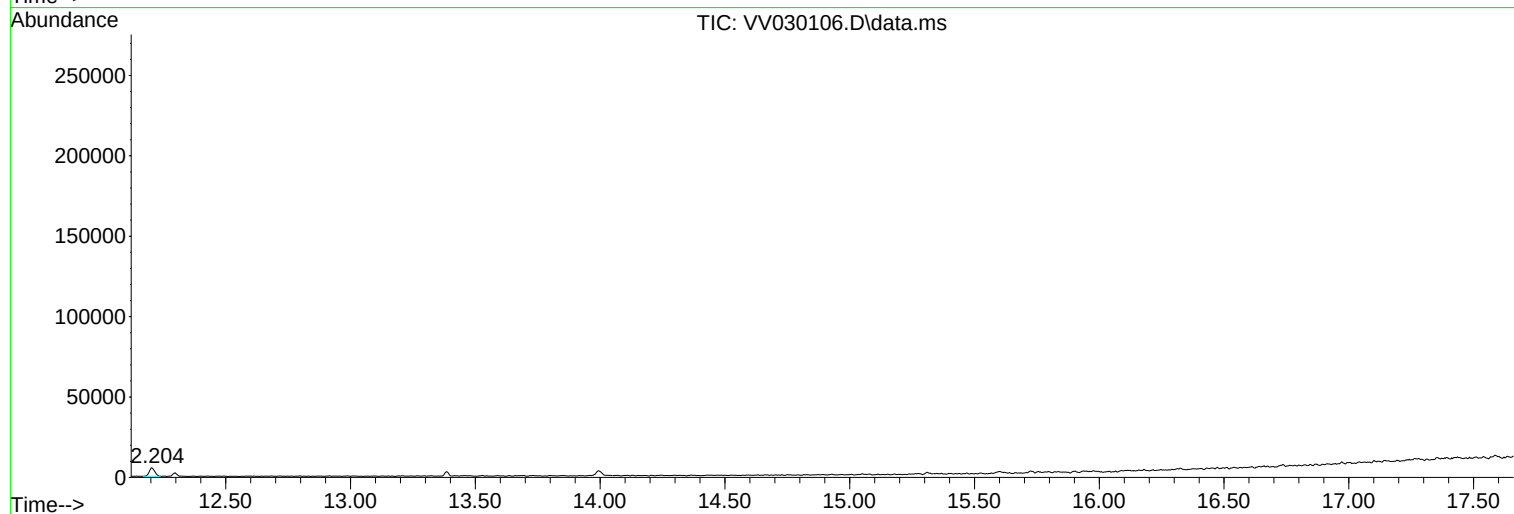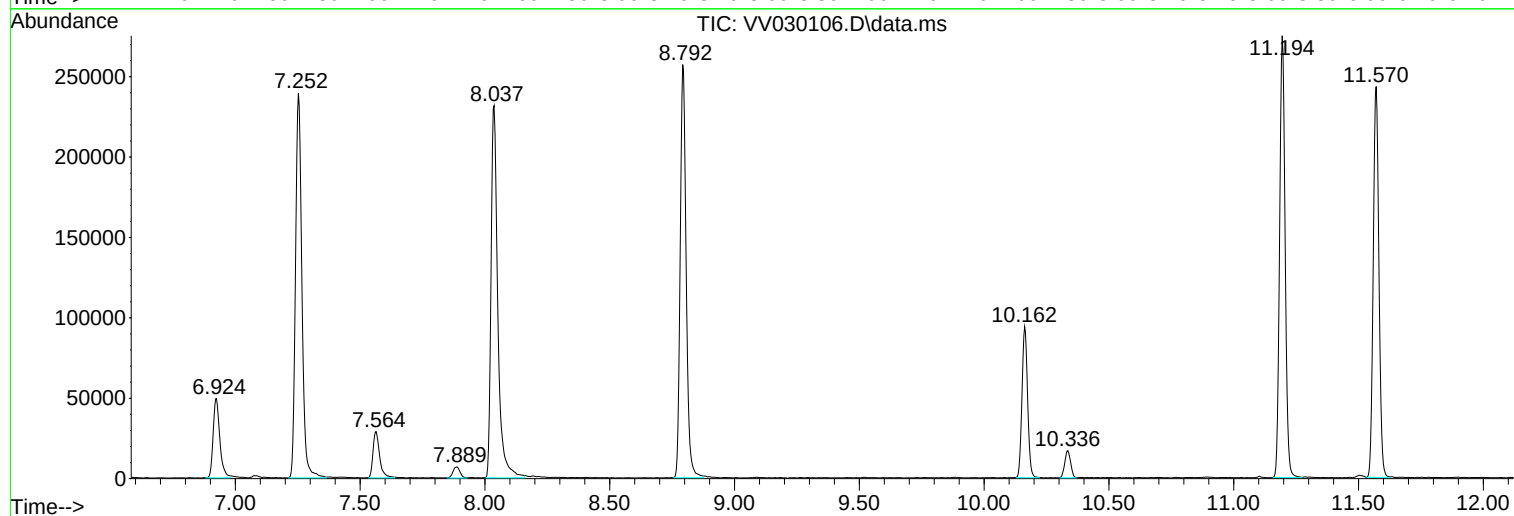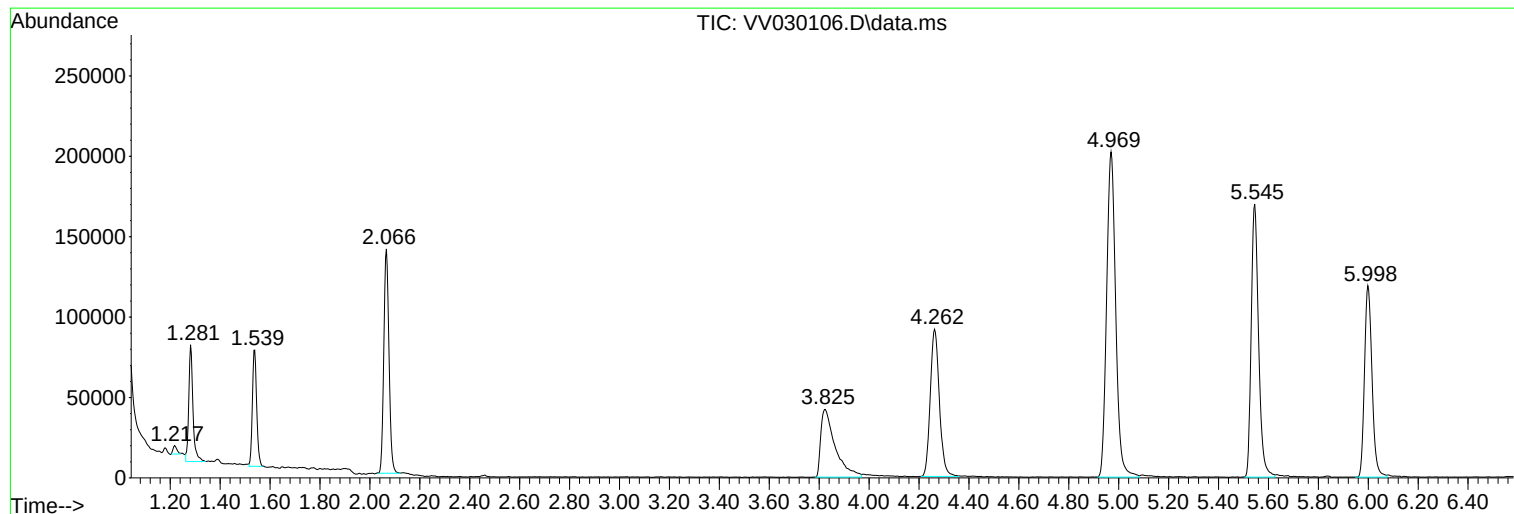

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030123\
Data File : VV030106.D
Acq On : 01 Mar 2023 13:40
Operator : SY/MD
Sample : 01729-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BZ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030123\
Data File : VV030106.D
Acq On : 01 Mar 2023 13:40
Operator : SY/MD
Sample : 01729-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BZ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc