

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030123\
 Data File : VV030107.D
 Acq On : 01 Mar 2023 14:04
 Operator : SY/MD
 Sample : 01729-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BZ6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030107.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.221	50	56	65	rBV2	7187	10543	1.95%	0.229%
2	1.282	69	75	94	rVB	79069	87368	16.15%	1.899%
3	1.539	147	155	170	rVB	76414	91111	16.85%	1.981%
4	2.066	308	319	335	rBV	149348	214707	39.70%	4.668%
5	3.818	853	864	907	rBV	48377	181843	33.62%	3.953%
6	4.262	985	1002	1039	rBV2	102623	284162	52.54%	6.178%
7	4.970	1203	1222	1246	rBV2	213675	540853	100.00%	11.759%
8	5.545	1388	1401	1424	rBV	174549	355458	65.72%	7.728%
9	5.998	1529	1542	1564	rBV	127999	263485	48.72%	5.728%
10	6.921	1818	1829	1860	rBV	52976	99918	18.47%	2.172%
11	7.252	1917	1932	1950	rBV	251826	441611	81.65%	9.601%
12	7.561	2019	2028	2050	rBV2	31629	56640	10.47%	1.231%
13	7.886	2117	2129	2145	rBV2	10846	20420	3.78%	0.444%
14	8.034	2165	2175	2204	rBV	247569	453363	83.82%	9.857%
15	8.793	2397	2411	2441	rBV	263704	437970	80.98%	9.522%
16	10.162	2823	2837	2853	rBV	100869	156110	28.86%	3.394%
17	10.336	2879	2891	2909	rVB	26943	45053	8.33%	0.979%
18	11.194	3146	3158	3186	rBV	280915	438393	81.06%	9.531%
19	11.571	3263	3275	3295	rBV	255486	404814	74.85%	8.801%
20	12.204	3460	3472	3489	rBV	10011	15809	2.92%	0.344%




Sum of corrected areas: 4599631

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030123\
Data File : VV030107.D
Acq On : 01 Mar 2023 14:04
Operator : SY/MD
Sample : 01729-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

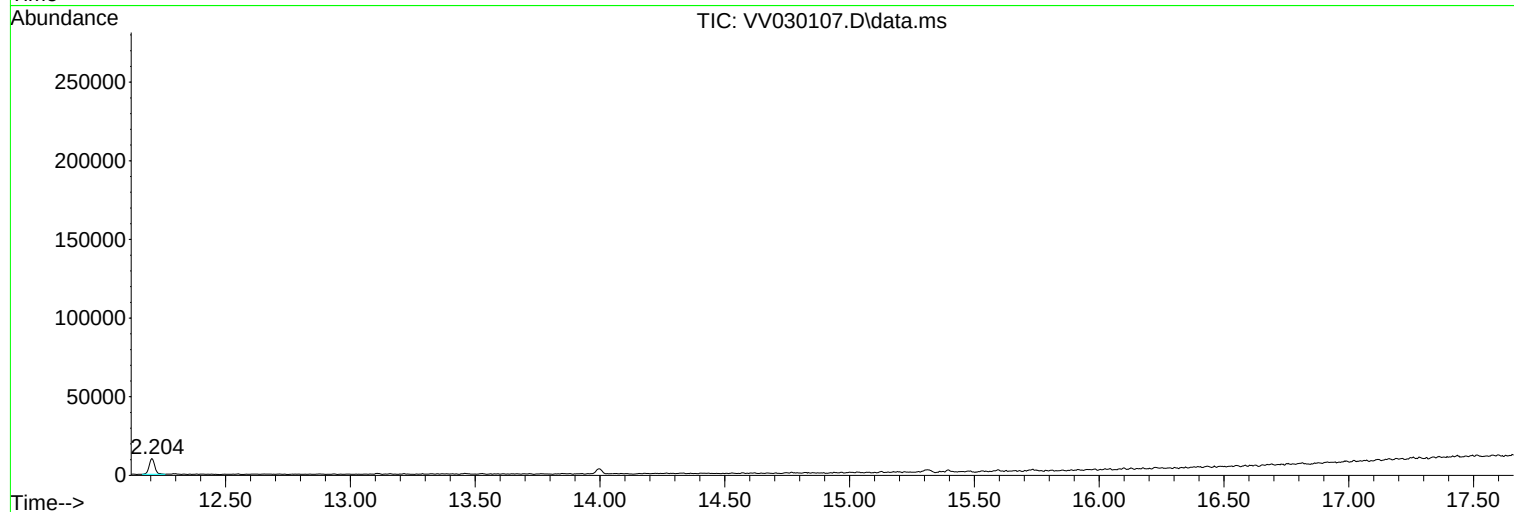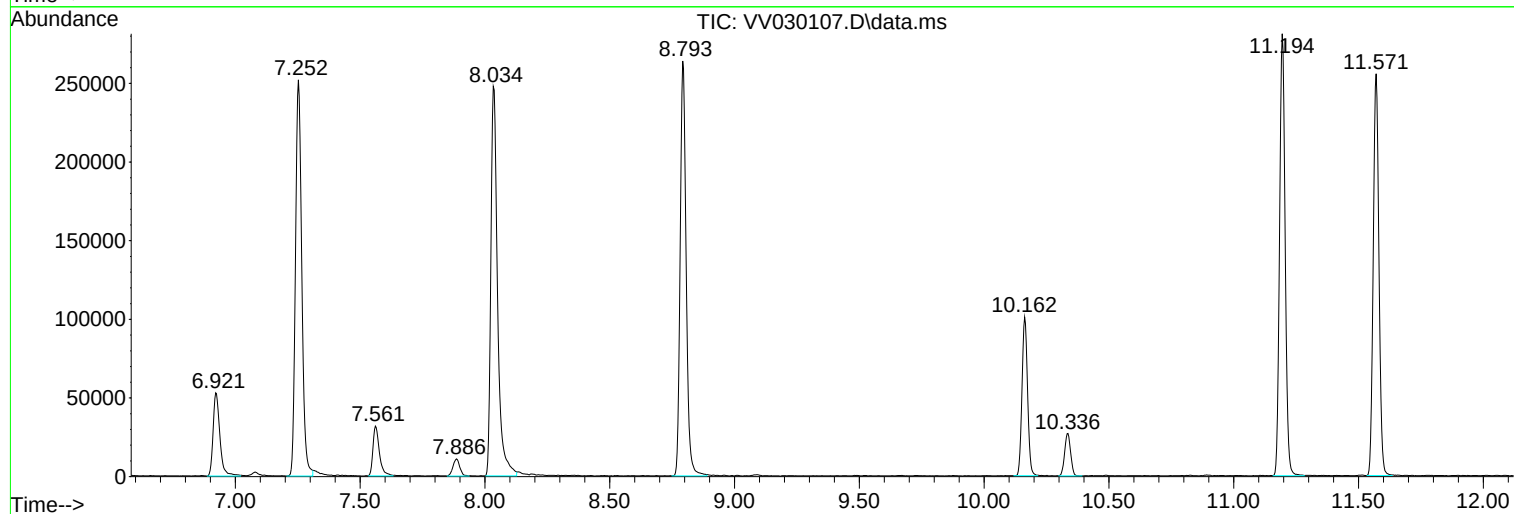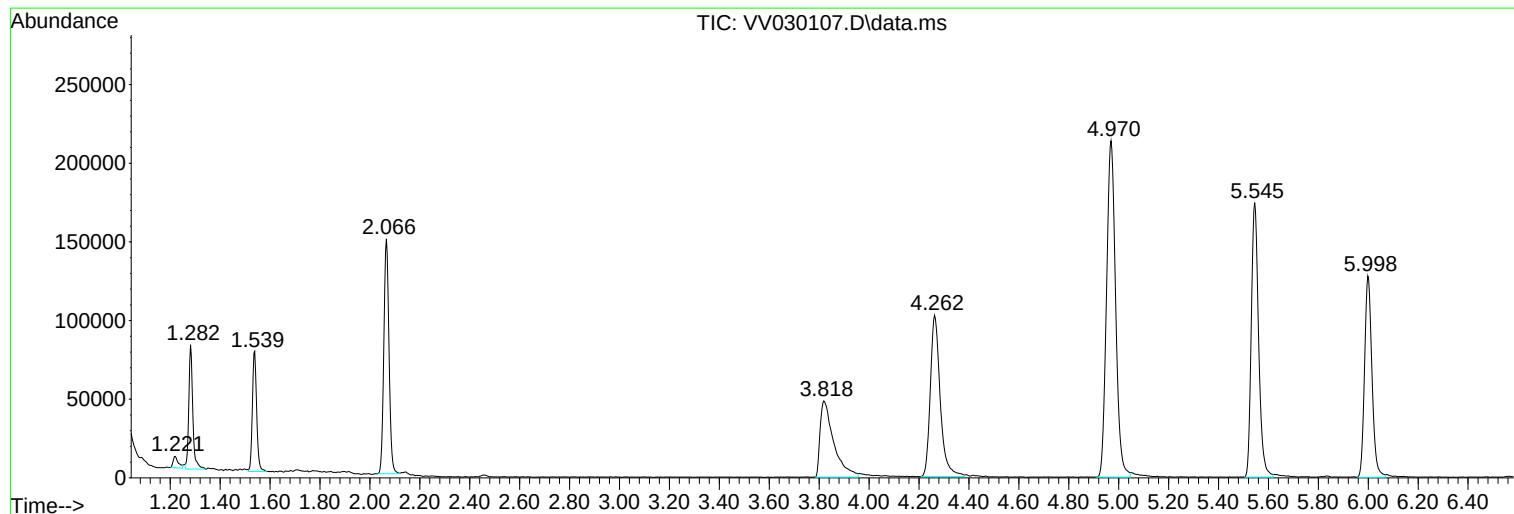

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030123\
Data File : VV030107.D
Acq On : 01 Mar 2023 14:04
Operator : SY/MD
Sample : 01729-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030123\
Data File : VV030107.D
Acq On : 01 Mar 2023 14:04
Operator : SY/MD
Sample : 01729-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc