

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030123\
 Data File : VV030108.D
 Acq On : 01 Mar 2023 14:26
 Operator : SY/MD
 Sample : 01729-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BZ8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030108.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	51	55	67	rBV	6792	10096	1.94%	0.227%
2	1.282	68	75	96	rVB	72300	84753	16.28%	1.909%
3	1.539	147	155	173	rVB	74956	87779	16.86%	1.977%
4	2.066	309	319	337	rBV	143219	207101	39.78%	4.664%
5	3.835	853	869	928	rBV2	41969	193024	37.07%	4.347%
6	4.265	986	1003	1038	rBV	96805	272629	52.36%	6.139%
7	4.973	1204	1223	1255	rBV2	204025	520656	100.00%	11.724%
8	5.545	1388	1401	1434	rBV	168032	349771	67.18%	7.876%
9	6.002	1529	1543	1568	rBV	120163	250760	48.16%	5.647%
10	6.924	1819	1830	1853	rBV2	50134	94231	18.10%	2.122%
11	7.256	1920	1933	1952	rBV	236484	423853	81.41%	9.545%
12	7.564	2019	2029	2048	rBV2	30563	54491	10.47%	1.227%
13	7.886	2118	2129	2145	rVB	7180	12943	2.49%	0.291%
14	8.037	2164	2176	2209	rBV	237554	447726	85.99%	10.082%
15	8.796	2399	2412	2445	rBV	250387	425742	81.77%	9.587%
16	10.162	2825	2837	2854	rBV	96491	152563	29.30%	3.436%
17	10.333	2879	2890	2904	rVB	16252	25633	4.92%	0.577%
18	11.194	3146	3158	3183	rBV	276005	425970	81.81%	9.592%
19	11.571	3263	3275	3294	rBV	246513	386737	74.28%	8.709%
20	12.204	3462	3472	3482	rBV2	5595	9040	1.74%	0.204%
21	13.998	4021	4030	4038	rVB	3572	5273	1.01%	0.119%




Sum of corrected areas: 4440771

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030123\
Data File : VV030108.D
Acq On : 01 Mar 2023 14:26
Operator : SY/MD
Sample : 01729-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BZ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

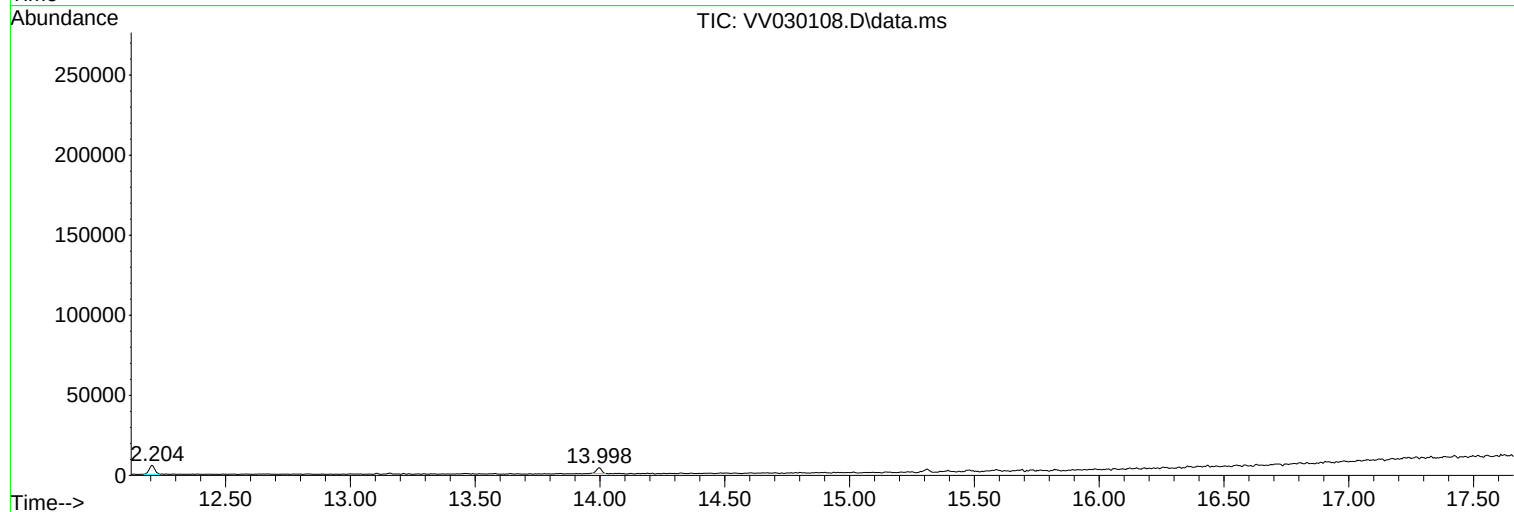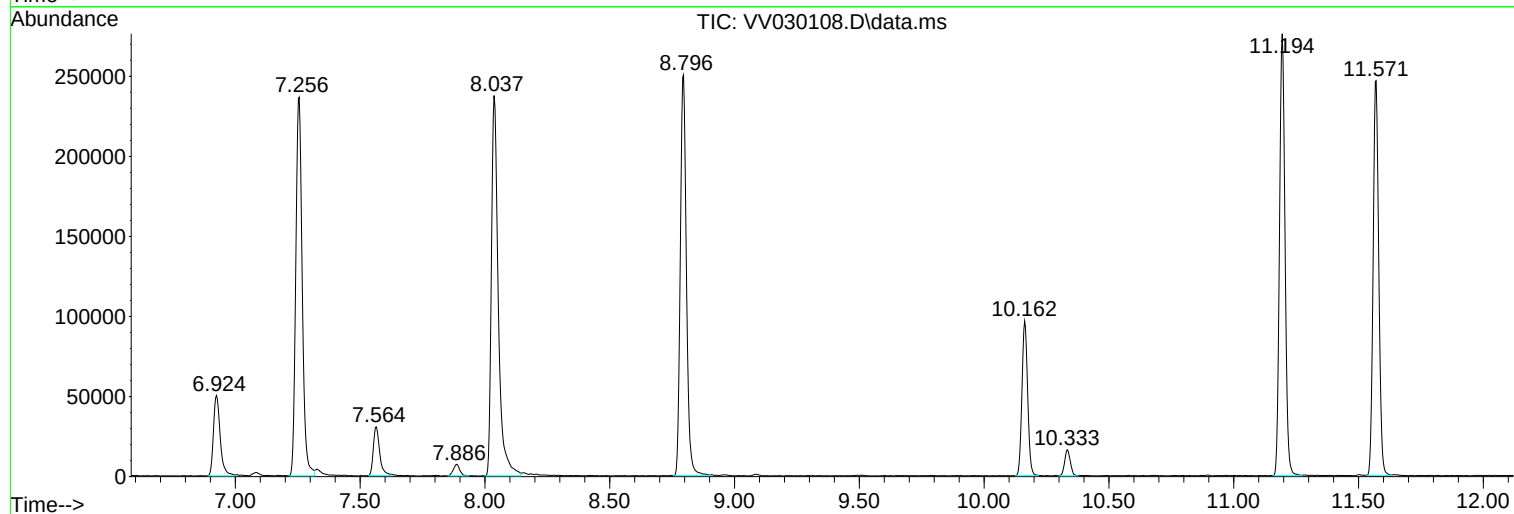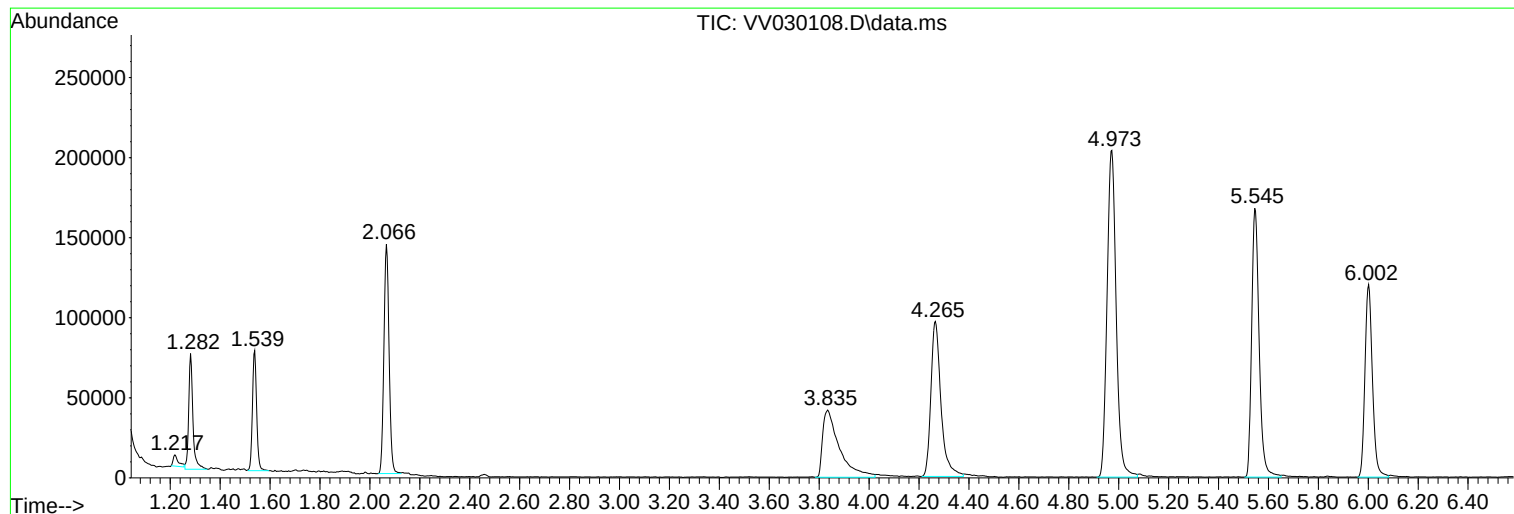

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030123\
Data File : VV030108.D
Acq On : 01 Mar 2023 14:26
Operator : SY/MD
Sample : 01729-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BZ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030123\
Data File : VV030108.D
Acq On : 01 Mar 2023 14:26
Operator : SY/MD
Sample : 01729-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BZ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------