
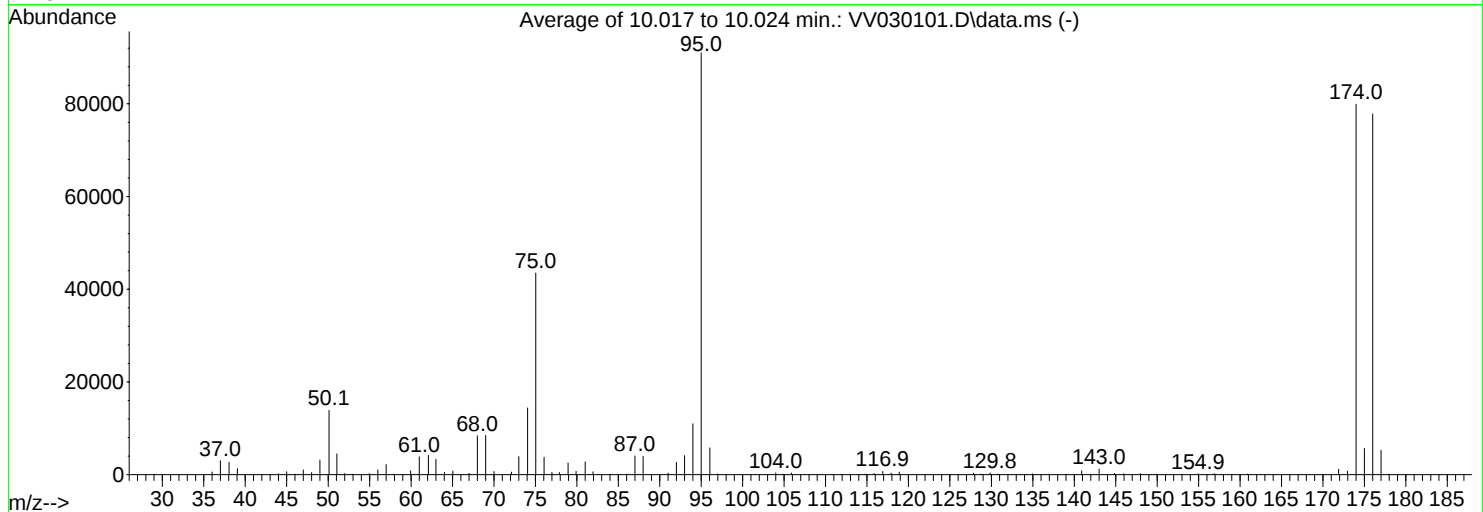


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030123\
Data File : VV030101.D
Acq On : 01 Mar 2023 11:07
Operator : SY/MD
Sample : BFB225
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB225

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Mar 03 03:28:37 2023

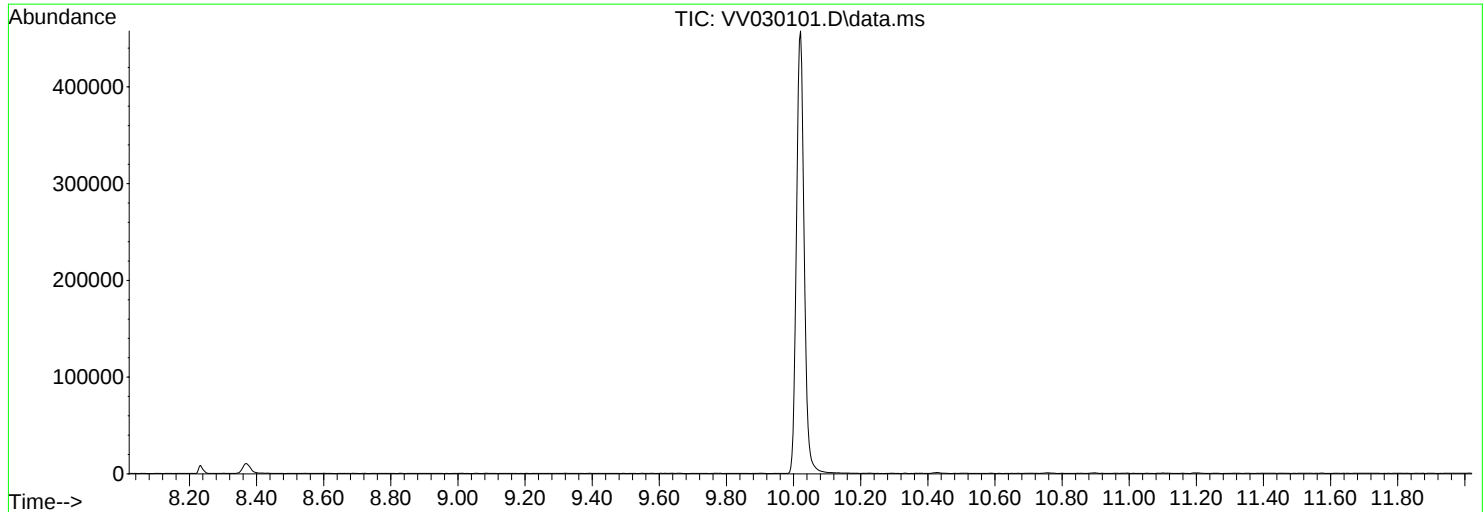

AutoFind: Scans 2792, 2793, 2794; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	13892	PASS
75	95	30	80	47.8	43504	PASS
95	95	100	100	100.0	91000	PASS
96	95	5	9	6.3	5756	PASS
173	174	0.00	2	1.0	770	PASS
174	95	50	120	87.8	79904	PASS
175	174	5	9	7.1	5679	PASS
176	174	95	105	97.4	77795	PASS
177	176	5	10	6.8	5253	PASS

m/z	Abundance
39.80	112.0
44.00	458.0

Instrument :
MSVOA_V
ClientSampleId :
BFB225

m/z	Abundance
36.00	571.0
37.00	3148.0
38.00	2691.0
39.10	1407.0
40.00	216.0
44.00	650.0
45.00	659.0
46.00	113.0
47.00	1107.0
48.00	495.0
49.00	3292.0
50.10	14545.0
51.00	4693.0
52.00	237.0
52.90	144.0
55.00	214.0
56.00	1057.0
57.00	2292.0
57.90	126.0
59.90	880.0
61.00	4113.0
62.10	4306.0
63.00	3428.0
64.00	536.0
65.10	784.0
67.00	243.0
68.00	8590.0
69.00	8706.0
70.00	779.0
72.10	545.0
73.00	4111.0
74.10	14826.0
75.00	43832.0
76.00	3886.0
77.00	516.0
77.90	455.0
78.90	2632.0
79.90	743.0
81.00	2830.0
81.90	564.0
82.90	129.0
86.00	209.0
87.00	4072.0
88.00	3971.0
91.00	327.0
92.00	2820.0
93.00	4199.0
94.00	11185.0
95.00	92288.0
96.10	6150.0
97.00	194.0
104.00	390.0
104.90	156.0
105.90	352.0
114.90	151.0
115.80	299.0
116.90	734.0
117.90	366.0
118.90	581.0
127.80	333.0
128.70	165.0
129.90	370.0
130.80	172.0
135.00	168.0
137.00	117.0
140.90	849.0
142.00	135.0
143.00	1247.0
144.90	280.0
145.90	190.0
148.00	235.0
150.00	147.0
155.00	236.0
156.90	218.0
160.90	126.0
170.90	132.0
171.90	1251.0
172.90	816.0
174.00	79200.0
175.00	5923.0
176.00	77024.0
177.00	5433.0
178.00	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB225

m/z	Abundance
36.00	600.0
37.00	3064.0
38.00	2711.0
39.10	1373.0
40.00	196.0
44.00	685.0
45.00	620.0
46.00	118.0
47.00	1034.0
48.00	469.0
49.00	3267.0
50.10	14318.0
51.10	4641.0
52.00	237.0
52.90	133.0
54.90	247.0
56.00	987.0
57.00	2262.0
57.90	157.0
60.00	868.0
61.00	3907.0
62.10	4353.0
63.00	3516.0
64.00	464.0
65.00	840.0
67.00	268.0
68.00	8623.0
69.00	8836.0
70.00	714.0
72.10	577.0
73.00	4051.0
74.10	14847.0
75.10	45056.0
76.10	3871.0
77.00	512.0
77.90	471.0
78.90	2553.0
79.90	766.0
81.00	2851.0
81.90	656.0
86.00	160.0
87.00	4158.0
88.00	4139.0
91.00	358.0
92.00	2784.0
93.00	4258.0
94.00	11367.0
95.00	94024.0
96.10	5942.0
97.00	195.0
104.00	414.0
104.80	142.0
105.90	375.0
111.90	101.0
112.90	119.0
114.80	135.0
115.90	292.0
116.90	714.0
117.90	372.0
118.90	587.0
127.80	327.0
128.70	159.0
129.80	398.0
130.80	165.0
134.90	179.0
137.00	135.0
140.90	864.0
141.90	117.0
143.00	1268.0
144.90	267.0
146.00	202.0
148.00	263.0
150.00	153.0
155.00	219.0
156.90	219.0
158.90	109.0
160.90	143.0
171.90	1208.0
173.00	763.0
174.00	82488.0
175.00	5862.0
176.00	80344.0
177.00	5418.0
177.90	128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB225

m/z	Abundance
36.00	566.0
37.00	2799.0
38.10	2603.0
39.00	1182.0
40.00	172.0
44.00	704.0
45.00	570.0
46.00	116.0
47.00	881.0
48.00	410.0
49.00	2899.0
50.10	12814.0
51.10	4142.0
52.00	211.0
54.90	254.0
56.00	930.0
57.00	1990.0
58.00	141.0
60.00	764.0
61.00	3434.0
62.10	3853.0
63.00	3049.0
64.10	428.0
65.00	790.0
67.00	288.0
68.00	7957.0
69.00	7986.0
70.00	566.0
72.10	506.0
73.00	3552.0
74.00	13554.0
75.10	41624.0
76.10	3481.0
77.00	524.0
77.90	425.0
79.00	2358.0
79.90	719.0
81.00	2638.0
82.00	622.0
86.00	116.0
87.00	3852.0
88.00	3754.0
91.00	314.0
92.00	2428.0
93.00	3847.0
94.00	10374.0
95.00	86688.0
96.00	5176.0
97.00	174.0
104.00	391.0
104.80	127.0
105.90	351.0
110.80	102.0
111.80	115.0
113.00	112.0
114.80	117.0
115.90	293.0
116.90	650.0
117.90	337.0
118.90	525.0
127.90	313.0
128.80	123.0
129.80	351.0
130.80	140.0
134.90	192.0
136.90	128.0
140.90	820.0
143.00	1144.0
144.80	247.0
146.00	181.0
148.00	243.0
149.90	116.0
154.80	195.0
156.90	193.0
158.90	115.0
160.90	113.0
171.90	1056.0
173.00	730.0
174.00	78024.0
175.00	5251.0
176.00	76016.0
177.00	4907.0
177.90	151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB225