

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030124\
 Data File : VV034489.D
 Acq On : 01 Mar 2024 10:13
 Operator : SY/MD
 Sample : VV0301WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK235

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034489.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	92	rVB	196764	210184	15.28%	2.036%
2	1.536	146	154	171	rVB	177535	200216	14.56%	1.940%
3	2.060	306	317	334	rBV	334357	491803	35.76%	4.765%
4	2.246	371	375	383	rVB2	815	931	0.07%	0.009%
5	2.404	420	424	431	rVV3	444	496	0.04%	0.005%
6	2.455	431	440	451	rVB2	2080	3847	0.28%	0.037%
7	2.696	512	515	517	rVV2	357	218	0.02%	0.002%
8	2.709	517	519	524	rVB2	550	388	0.03%	0.004%
9	2.786	540	543	549	rVV2	263	280	0.02%	0.003%
10	2.992	602	607	612	rBV2	226	206	0.01%	0.002%
11	3.140	648	653	660	rBV2	146	219	0.02%	0.002%
12	3.793	847	856	893	rBV	110350	320138	23.28%	3.102%
13	4.249	981	998	1023	rBV	219789	562072	40.87%	5.446%
14	4.481	1068	1070	1076	rVB3	593	363	0.03%	0.004%
15	4.603	1106	1108	1110	rBV	388	202	0.01%	0.002%
16	4.677	1129	1131	1136	rBV4	329	237	0.02%	0.002%
17	4.738	1147	1150	1155	rVB2	514	354	0.03%	0.003%
18	4.777	1157	1162	1165	rBV2	267	284	0.02%	0.003%
19	4.793	1165	1167	1172	rVB3	286	210	0.02%	0.002%
20	4.957	1202	1218	1254	rBV2	518293	1375173	100.00%	13.324%
21	5.195	1290	1292	1297	rVB4	470	405	0.03%	0.004%
22	5.285	1316	1320	1323	rBV3	360	283	0.02%	0.003%
23	5.532	1386	1397	1430	rBV	363662	759905	55.26%	7.363%
24	5.828	1479	1489	1516	rVB3	13463	30762	2.24%	0.298%
25	5.937	1519	1523	1526	rBV2	388	356	0.03%	0.003%
26	5.989	1526	1539	1570	rBV	299223	624402	45.41%	6.050%
27	6.137	1583	1585	1589	rVB2	576	305	0.02%	0.003%
28	6.207	1605	1607	1613	rVB2	476	399	0.03%	0.004%
29	6.339	1644	1648	1650	rBV	246	197	0.01%	0.002%
30	6.474	1687	1690	1696	rVB2	350	381	0.03%	0.004%
31	6.510	1696	1701	1704	rBV2	269	316	0.02%	0.003%
32	6.551	1708	1714	1719	rVV2	191	274	0.02%	0.003%
33	6.593	1720	1727	1729	rVV3	767	723	0.05%	0.007%
34	6.606	1729	1731	1734	rVV2	669	464	0.03%	0.004%
35	6.622	1734	1736	1739	rVV2	487	354	0.03%	0.003%
36	6.645	1742	1743	1750	rVB2	367	264	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030124\
 Data File : VV034489.D
 Acq On : 01 Mar 2024 10:13
 Operator : SY/MD
 Sample : VV0301WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK235

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.912	1816	1826	1853	rBV	160032	301647	21.94%	2.923%
38	7.140	1889	1897	1899	rBV3	830	897	0.07%	0.009%
39	7.243	1917	1929	1955	rBV	595993	1050019	76.36%	10.173%
40	7.551	2016	2025	2060	rBV	108989	203347	14.79%	1.970%
41	7.780	2094	2096	2100	rVB3	366	246	0.02%	0.002%
42	7.831	2107	2112	2116	rBV2	369	440	0.03%	0.004%
43	7.879	2124	2127	2131	rVB2	428	326	0.02%	0.003%
44	8.024	2162	2172	2214	rBV	421817	777443	56.53%	7.533%
45	8.355	2274	2275	2277	rBV	528	249	0.02%	0.002%
46	8.407	2288	2291	2293	rBV2	380	247	0.02%	0.002%
47	8.506	2320	2322	2328	rVB3	584	495	0.04%	0.005%
48	8.538	2328	2332	2336	rBV3	300	329	0.02%	0.003%
49	8.641	2361	2364	2368	rVB2	315	278	0.02%	0.003%
50	8.741	2391	2395	2398	rBV3	382	313	0.02%	0.003%
51	8.783	2398	2408	2432	rBV	549458	902533	65.63%	8.745%
52	9.101	2501	2507	2510	rBV3	354	385	0.03%	0.004%
53	9.275	2554	2561	2564	rBV2	185	239	0.02%	0.002%
54	9.493	2621	2629	2634	rBV2	551	675	0.05%	0.007%
55	9.802	2722	2725	2731	rVB	262	238	0.02%	0.002%
56	9.837	2731	2736	2740	rBV	308	334	0.02%	0.003%
57	9.937	2762	2767	2770	rBV	254	242	0.02%	0.002%
58	10.153	2822	2834	2858	rBV	405244	645092	46.91%	6.250%
59	10.281	2872	2874	2880	rVB2	264	236	0.02%	0.002%
60	10.329	2880	2889	2895	rBV4	865	1346	0.10%	0.013%
61	10.374	2897	2903	2908	rBV2	348	402	0.03%	0.004%
62	10.484	2933	2937	2943	rVB3	362	398	0.03%	0.004%
63	10.725	3008	3012	3016	rBV2	401	323	0.02%	0.003%
64	10.863	3050	3055	3057	rBV	334	288	0.02%	0.003%
65	10.969	3081	3088	3093	rBV	311	347	0.03%	0.003%
66	11.140	3136	3141	3144	rBV3	381	415	0.03%	0.004%
67	11.185	3144	3155	3180	rBV	549411	864188	62.84%	8.373%
68	11.336	3200	3202	3207	rBV2	378	328	0.02%	0.003%
69	11.455	3235	3239	3241	rBV2	354	252	0.02%	0.002%
70	11.487	3245	3249	3253	rBV2	308	259	0.02%	0.003%
71	11.558	3259	3271	3293	rBV	615373	961844	69.94%	9.319%
72	11.767	3332	3336	3340	rVB4	413	407	0.03%	0.004%
73	11.886	3370	3373	3378	rBV2	228	220	0.02%	0.002%
74	12.037	3417	3420	3425	rVB2	392	226	0.02%	0.002%
75	12.104	3436	3441	3445	rBV2	267	307	0.02%	0.003%
76	12.191	3463	3468	3476	rBV	757	886	0.06%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030124\
 Data File : VV034489.D
 Acq On : 01 Mar 2024 10:13
 Operator : SY/MD
 Sample : VV0301WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK235

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	12.304	3500	3503	3507	rBV2	210	198	0.01%	0.002%
78	12.461	3549	3552	3559	rVB2	220	245	0.02%	0.002%
79	12.509	3563	3567	3571	rBV	231	269	0.02%	0.003%
80	12.686	3619	3622	3624	rBV	386	202	0.01%	0.002%
81	12.812	3657	3661	3664	rBV	451	342	0.02%	0.003%
82	12.863	3672	3677	3683	rBV2	420	540	0.04%	0.005%
83	12.985	3712	3715	3718	rVB	367	245	0.02%	0.002%
84	13.162	3768	3770	3775	rVB2	374	234	0.02%	0.002%
85	13.210	3779	3785	3794	rVB4	1134	1500	0.11%	0.015%
86	13.310	3812	3816	3820	rBV	391	264	0.02%	0.003%
87	13.342	3823	3826	3829	rBV2	297	237	0.02%	0.002%
88	13.455	3852	3861	3869	rBV5	2454	4155	0.30%	0.040%
89	13.628	3909	3915	3919	rBV3	429	487	0.04%	0.005%
90	13.683	3927	3932	3939	rVB4	1058	1326	0.10%	0.013%
91	13.802	3967	3969	3973	rBV3	301	250	0.02%	0.002%
92	13.866	3986	3989	3993	rVB3	366	283	0.02%	0.003%
93	14.037	4035	4042	4044	rBV2	538	510	0.04%	0.005%
94	14.178	4083	4086	4089	rVB3	335	258	0.02%	0.002%
95	14.448	4165	4170	4175	rBV3	711	732	0.05%	0.007%
96	14.895	4306	4309	4312	rBV5	484	319	0.02%	0.003%
97	14.927	4317	4319	4322	rVB2	627	262	0.02%	0.003%
98	15.114	4374	4377	4380	rBV3	822	642	0.05%	0.006%
99	15.493	4492	4495	4499	rBV4	848	804	0.06%	0.008%
100	15.525	4503	4505	4507	rBV3	923	531	0.04%	0.005%




Sum of corrected areas: 10321132

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030124\
Data File : VV034489.D
Acq On : 01 Mar 2024 10:13
Operator : SY/MD
Sample : VV0301WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK235

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

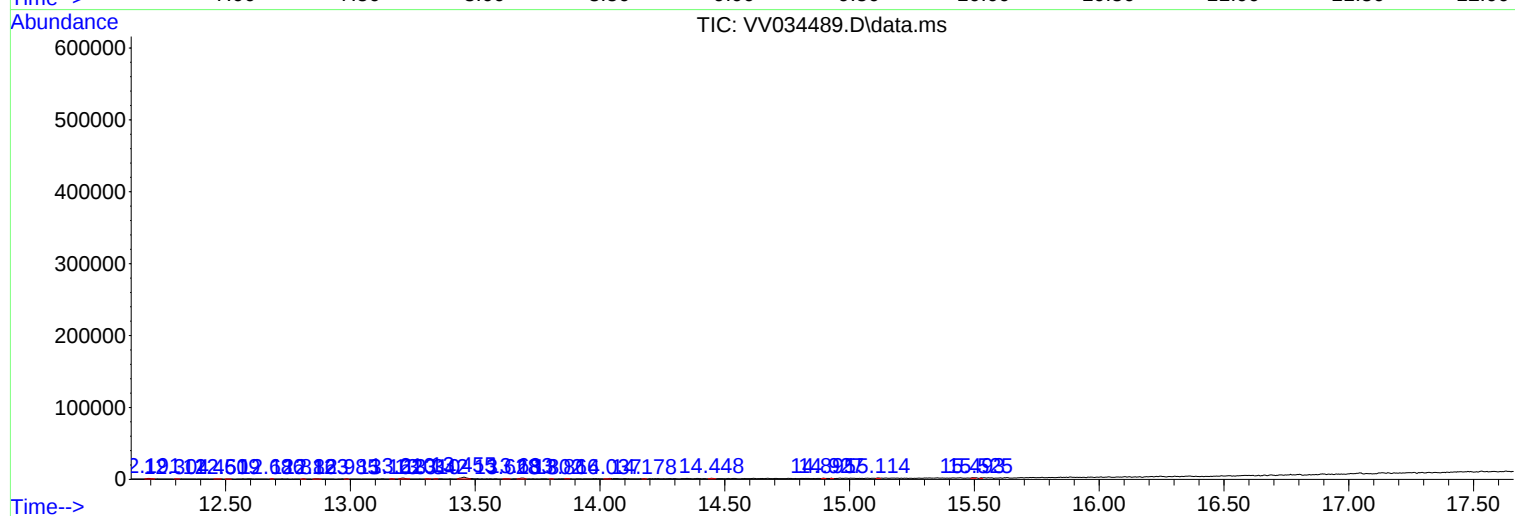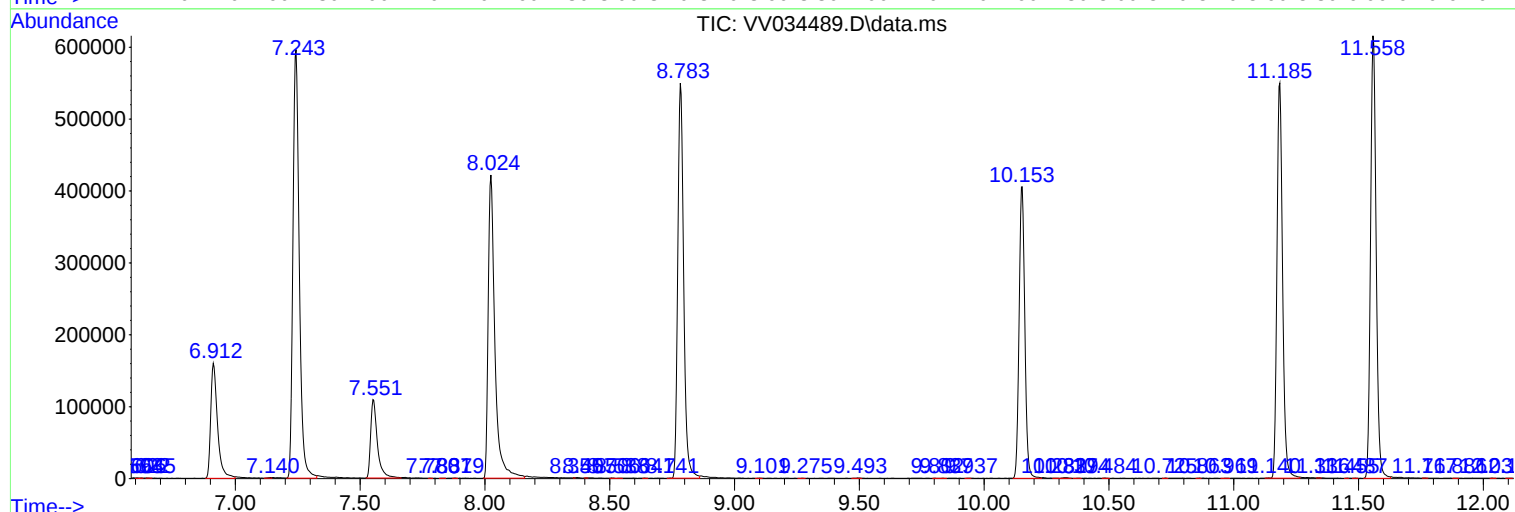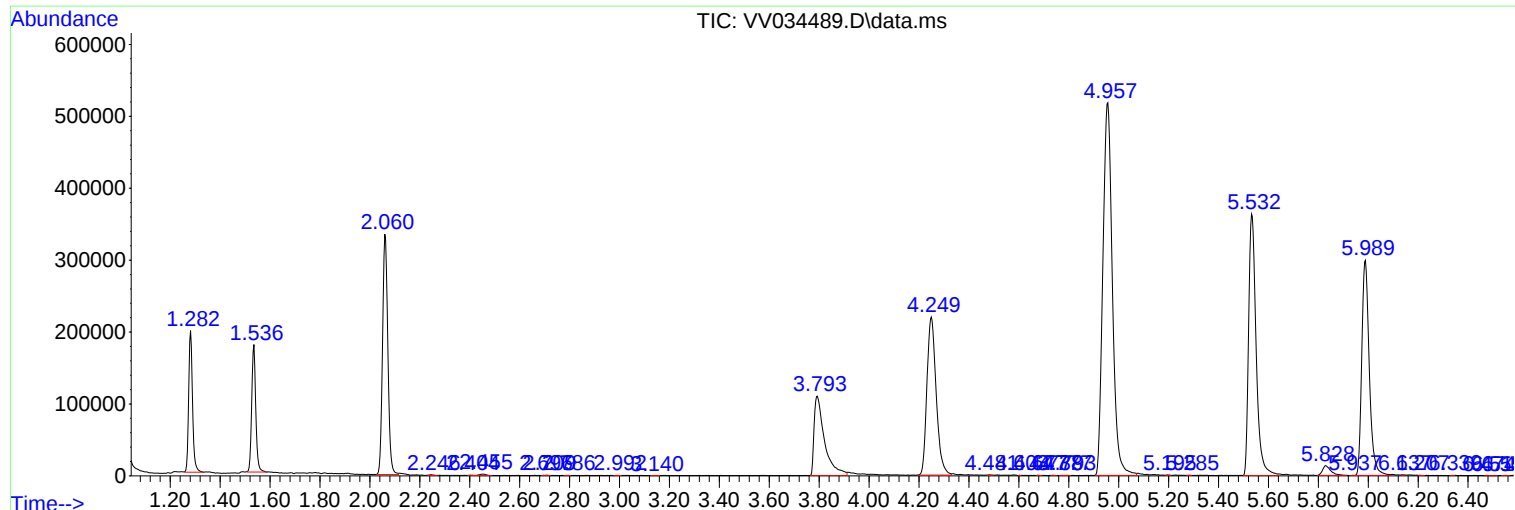

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030124\
Data File : VV034489.D
Acq On : 01 Mar 2024 10:13
Operator : SY/MD
Sample : VV0301WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK235

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030124\
Data File : VV034489.D
Acq On : 01 Mar 2024 10:13
Operator : SY/MD
Sample : VV0301WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK235

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------