

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030124\
 Data File : VV034490.D
 Acq On : 01 Mar 2024 10:37
 Operator : SY/MD
 Sample : P1642-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034490.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	93	rVB	181259	197350	15.33%	2.049%
2	1.532	146	153	175	rVB	159670	187123	14.54%	1.942%
3	2.060	307	317	336	rBV	309203	447647	34.78%	4.647%
4	2.378	414	416	419	rBV2	301	110	0.01%	0.001%
5	2.416	425	428	431	rBV	314	178	0.01%	0.002%
6	2.449	431	438	446	rVV5	1828	3139	0.24%	0.033%
7	2.561	471	473	476	rVB	393	232	0.02%	0.002%
8	2.625	490	493	495	rBV	206	110	0.01%	0.001%
9	2.799	543	547	549	rBV2	151	145	0.01%	0.002%
10	2.998	606	609	614	rVB	182	143	0.01%	0.001%
11	3.027	615	618	619	rBV2	192	92	0.01%	0.001%
12	3.146	651	655	657	rBV	133	100	0.01%	0.001%
13	3.162	657	660	663	rVV2	192	134	0.01%	0.001%
14	3.233	675	682	685	rBV2	243	334	0.03%	0.003%
15	3.371	721	725	729	rVB2	143	124	0.01%	0.001%
16	3.407	732	736	739	rBV2	186	122	0.01%	0.001%
17	3.436	742	745	750	rVB2	220	153	0.01%	0.002%
18	3.564	783	785	789	rVB	212	100	0.01%	0.001%
19	3.613	797	800	803	rVB	185	110	0.01%	0.001%
20	3.638	805	808	815	rVB2	183	218	0.02%	0.002%
21	3.789	846	855	888	rBV	108658	305456	23.74%	3.171%
22	4.246	983	997	1028	rBV	204112	517324	40.20%	5.370%
23	4.654	1122	1124	1126	rBV2	200	113	0.01%	0.001%
24	4.722	1143	1145	1148	rVB2	495	233	0.02%	0.002%
25	4.764	1155	1158	1162	rVB2	239	206	0.02%	0.002%
26	4.789	1162	1166	1169	rBV2	240	249	0.02%	0.003%
27	4.883	1193	1195	1199	rVB	276	157	0.01%	0.002%
28	4.953	1199	1217	1246	rBV2	481519	1286943	100.00%	13.359%
29	5.336	1333	1336	1337	rBV2	317	164	0.01%	0.002%
30	5.368	1344	1346	1348	rBV	256	129	0.01%	0.001%
31	5.397	1352	1355	1356	rVB	220	98	0.01%	0.001%
32	5.420	1359	1362	1366	rVB2	181	138	0.01%	0.001%
33	5.439	1366	1368	1370	rBV3	357	189	0.01%	0.002%
34	5.484	1380	1382	1386	rVB2	207	110	0.01%	0.001%
35	5.532	1386	1397	1424	rBV	340075	699571	54.36%	7.262%
36	5.831	1479	1490	1503	rBV4	12355	26011	2.02%	0.270%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030124\
 Data File : VV034490.D
 Acq On : 01 Mar 2024 10:37
 Operator : SY/MD
 Sample : P1642-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	5.918	1515	1517	1519	rVB	268	116	0.01%	0.001%
38	5.937	1521	1523	1526	rBV2	235	127	0.01%	0.001%
39	5.985	1526	1538	1568	rBV	278246	582136	45.23%	6.043%
40	6.210	1607	1608	1611	rVB2	405	167	0.01%	0.002%
41	6.252	1619	1621	1624	rBV3	255	138	0.01%	0.001%
42	6.288	1630	1632	1639	rVB3	184	195	0.02%	0.002%
43	6.333	1639	1646	1650	rVB2	347	354	0.03%	0.004%
44	6.403	1664	1668	1669	rBV2	142	97	0.01%	0.001%
45	6.564	1714	1718	1721	rBV	326	236	0.02%	0.002%
46	6.593	1721	1727	1729	rBV4	719	708	0.06%	0.007%
47	6.722	1764	1767	1770	rBV	260	207	0.02%	0.002%
48	6.809	1791	1794	1798	rVB	162	99	0.01%	0.001%
49	6.911	1816	1826	1868	rBV	149657	287775	22.36%	2.987%
50	7.243	1917	1929	1963	rBV	557319	981269	76.25%	10.186%
51	7.497	2006	2008	2010	rVB2	319	122	0.01%	0.001%
52	7.551	2016	2025	2045	rBV	103996	187015	14.53%	1.941%
53	7.802	2101	2103	2106	rBV	230	109	0.01%	0.001%
54	7.876	2117	2126	2132	rBV4	652	1083	0.08%	0.011%
55	8.024	2162	2172	2210	rBV	410403	743237	57.75%	7.715%
56	8.519	2324	2326	2329	rBV	278	147	0.01%	0.002%
57	8.648	2363	2366	2368	rBV	237	160	0.01%	0.002%
58	8.734	2391	2393	2397	rVB2	295	164	0.01%	0.002%
59	8.783	2397	2408	2436	rBV	510281	846697	65.79%	8.789%
60	9.062	2493	2495	2500	rVB2	275	148	0.01%	0.002%
61	9.091	2501	2504	2505	rBV	275	160	0.01%	0.002%
62	9.114	2508	2511	2513	rBV3	218	144	0.01%	0.001%
63	9.223	2543	2545	2550	rVB2	263	150	0.01%	0.002%
64	9.252	2550	2554	2557	rBV2	308	250	0.02%	0.003%
65	9.316	2569	2574	2575	rBV2	363	210	0.02%	0.002%
66	9.374	2591	2592	2596	rBV	159	113	0.01%	0.001%
67	9.432	2607	2610	2613	rBV	269	178	0.01%	0.002%
68	9.474	2619	2623	2628	rBV	200	224	0.02%	0.002%
69	9.529	2638	2640	2642	rBV	257	113	0.01%	0.001%
70	9.580	2651	2656	2659	rVB2	274	234	0.02%	0.002%
71	9.609	2659	2665	2667	rBV	335	281	0.02%	0.003%
72	9.722	2697	2700	2704	rBV2	219	185	0.01%	0.002%
73	9.953	2769	2772	2777	rVB	203	168	0.01%	0.002%
74	10.069	2806	2808	2812	rVB2	194	84	0.01%	0.001%
75	10.149	2822	2833	2862	rBV	392441	615694	47.84%	6.391%
76	10.313	2880	2884	2885	rBV2	447	291	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030124\
 Data File : VV034490.D
 Acq On : 01 Mar 2024 10:37
 Operator : SY/MD
 Sample : P1642-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.480	2933	2936	2940	rVB2	470	285	0.02%	0.003%
78	10.628	2978	2982	2987	rBV2	285	315	0.02%	0.003%
79	10.725	3006	3012	3017	rBV	353	403	0.03%	0.004%
80	10.770	3025	3026	3033	rBV	162	94	0.01%	0.001%
81	10.863	3049	3055	3060	rBV3	355	495	0.04%	0.005%
82	10.934	3074	3077	3079	rBV2	113	86	0.01%	0.001%
83	11.050	3110	3113	3115	rBV	155	97	0.01%	0.001%
84	11.098	3126	3128	3131	rBV	286	138	0.01%	0.001%
85	11.133	3136	3139	3142	rBV2	512	384	0.03%	0.004%
86	11.185	3144	3155	3176	rBV	509830	807562	62.75%	8.383%
87	11.474	3242	3245	3250	rVB2	268	172	0.01%	0.002%
88	11.558	3259	3271	3291	rBV	565576	895297	69.57%	9.294%
89	11.844	3357	3360	3362	rBV2	256	174	0.01%	0.002%
90	11.931	3379	3387	3390	rBV	397	483	0.04%	0.005%
91	12.165	3457	3460	3463	rBV	300	248	0.02%	0.003%
92	12.596	3591	3594	3601	rBV3	404	389	0.03%	0.004%
93	12.718	3629	3632	3634	rBV2	189	139	0.01%	0.001%
94	12.802	3655	3658	3660	rBV2	208	124	0.01%	0.001%
95	13.059	3736	3738	3740	rBV	247	128	0.01%	0.001%
96	13.091	3745	3748	3751	rBV3	262	175	0.01%	0.002%
97	13.358	3829	3831	3832	rBV	257	115	0.01%	0.001%
98	13.654	3921	3923	3924	rBV	289	144	0.01%	0.001%
99	13.683	3930	3932	3933	rBV	561	204	0.02%	0.002%
100	13.715	3939	3942	3943	rBV	327	180	0.01%	0.002%




Sum of corrected areas: 9633571

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030124\
Data File : VV034490.D
Acq On : 01 Mar 2024 10:37
Operator : SY/MD
Sample : P1642-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

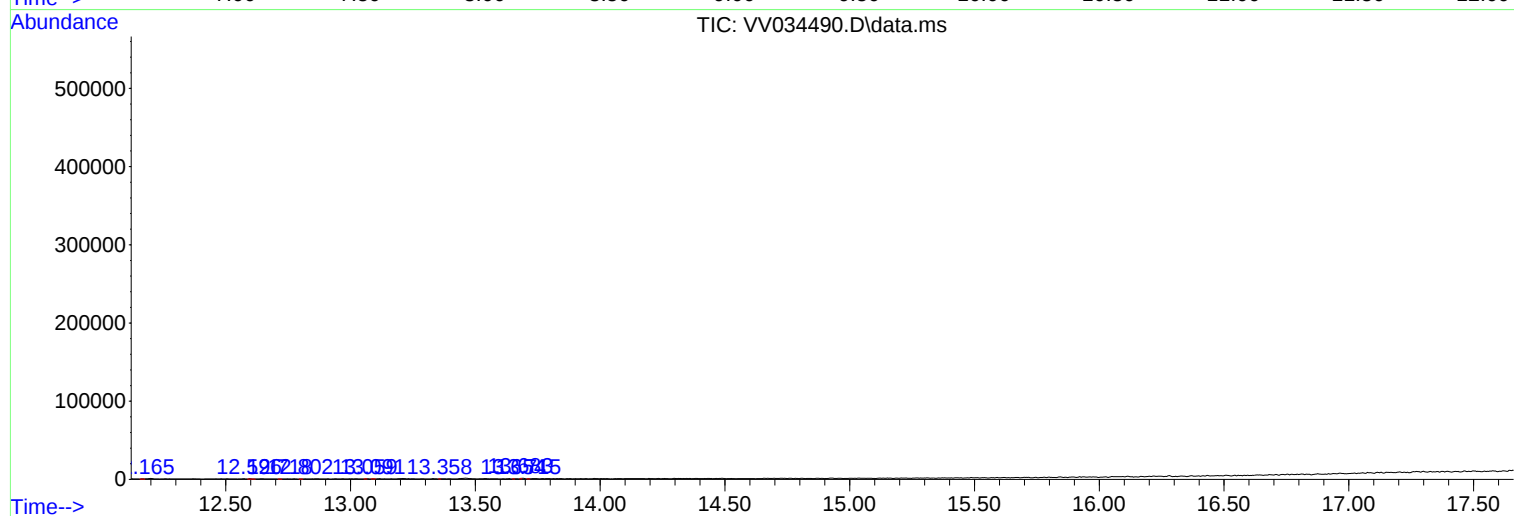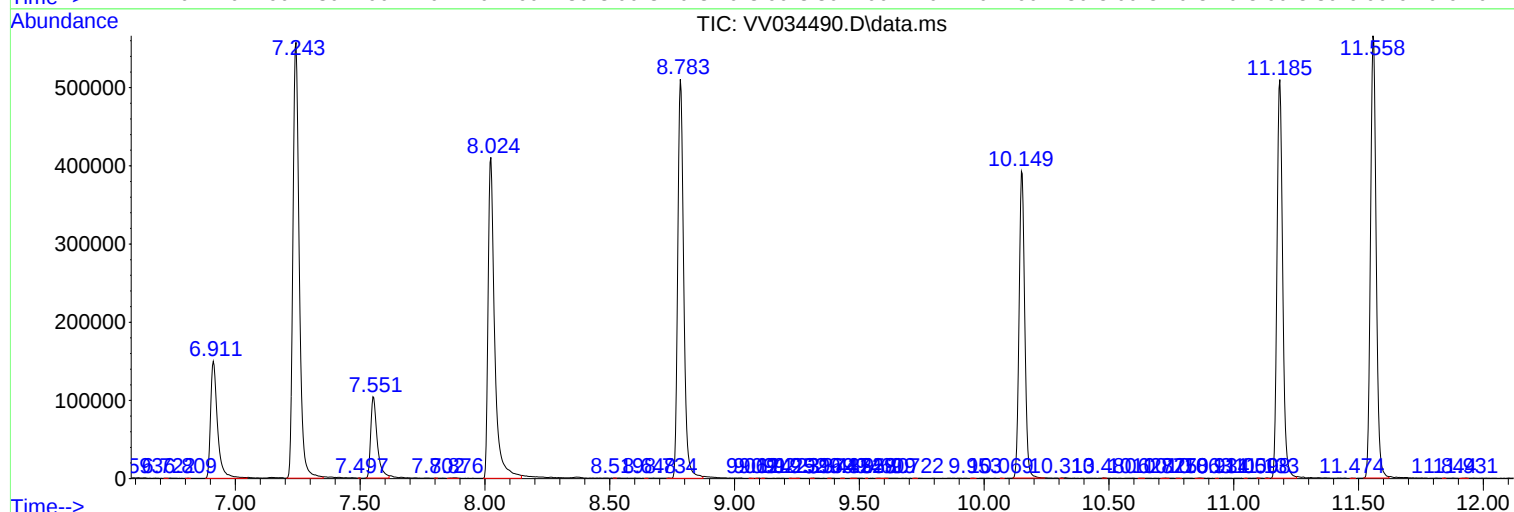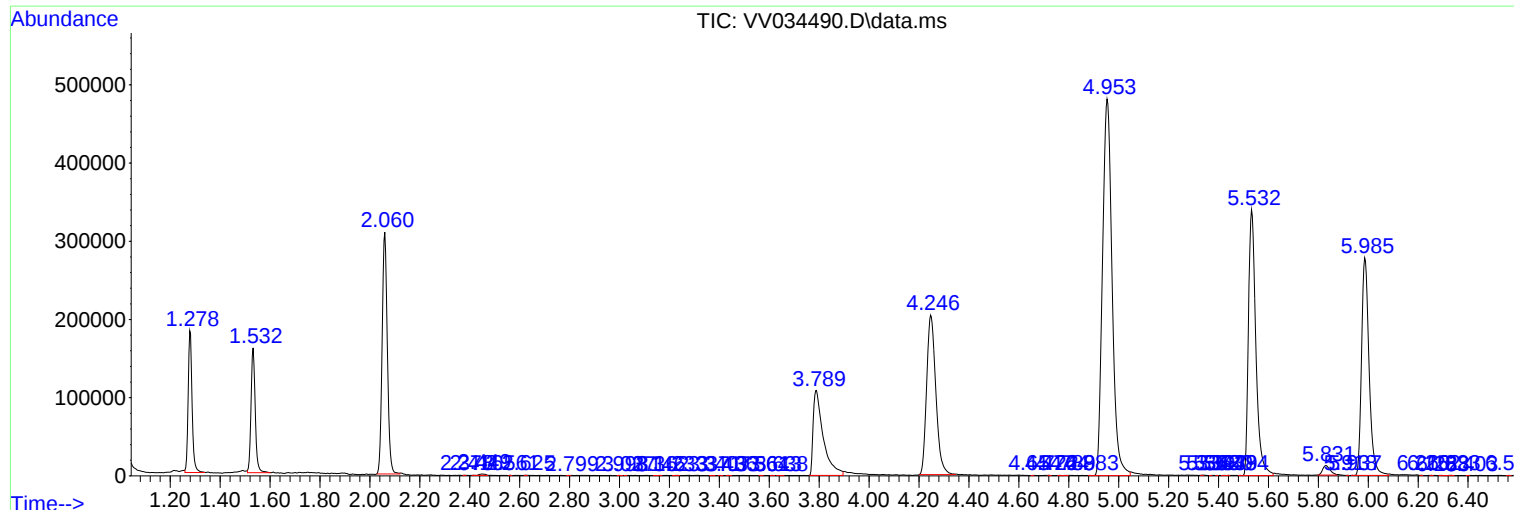

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030124\
Data File : VV034490.D
Acq On : 01 Mar 2024 10:37
Operator : SY/MD
Sample : P1642-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030124\
Data File : VV034490.D
Acq On : 01 Mar 2024 10:37
Operator : SY/MD
Sample : P1642-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc