


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030124\
Data File : VV034486.D
Acq On : 01 Mar 2024 08:31
Operator : SY/MD
Sample : BFB263
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB263

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Title : VOC Analysis
Last Update : Fri Mar 01 22:18:41 2024

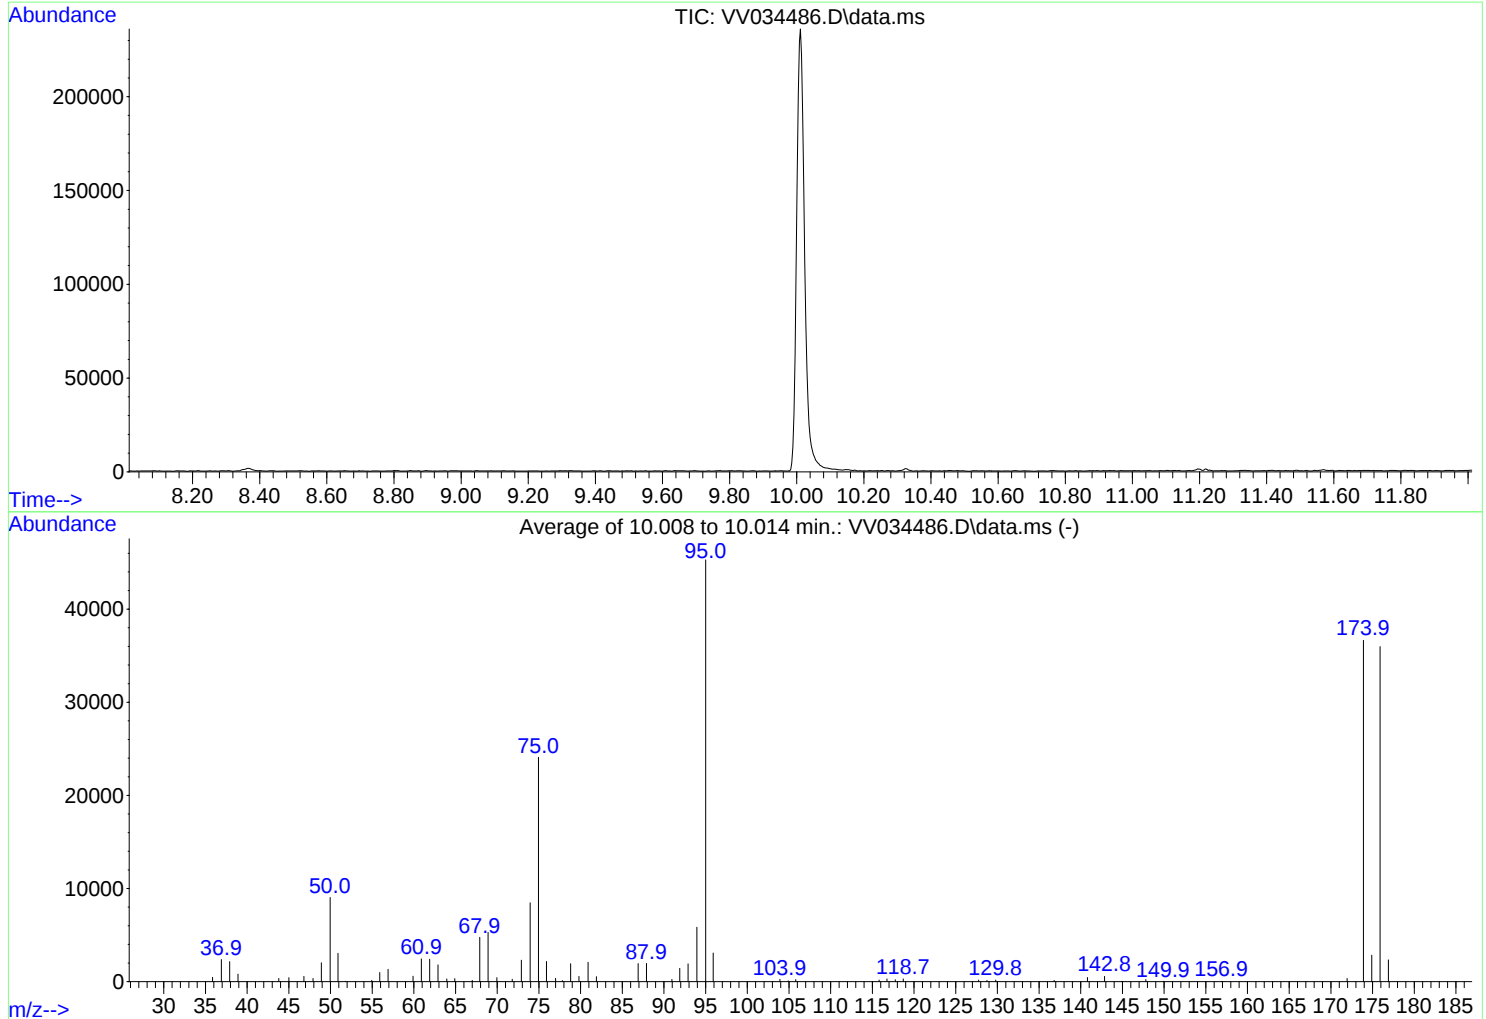

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.9	9036	PASS
75	95	30	80	53.2	24083	PASS
95	95	100	100	100.0	45296	PASS
96	95	5	9	6.8	3083	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.9	36656	PASS
175	174	5	9	7.8	2845	PASS
176	174	95	105	98.2	35984	PASS
177	176	5	10	6.5	2342	PASS

m/z	Abundance
35.90	518.0
36.90	2384.0
37.90	2288.0
38.90	790.0
39.80	306.0
43.90	520.0
45.00	377.0
46.80	606.0
47.90	340.0
48.90	2156.0
49.90	9258.0
50.90	3056.0
51.80	117.0
55.00	160.0
55.90	1085.0
56.90	1396.0
59.90	536.0
60.90	2403.0
61.90	2537.0
62.90	1895.0
64.00	306.0
64.90	345.0
67.00	113.0
67.90	4755.0
68.90	5294.0
70.00	422.0
71.80	274.0
72.90	2444.0
74.00	8435.0
74.90	24344.0
75.90	2164.0
77.00	350.0
77.90	123.0
78.80	1947.0
79.80	522.0
80.90	2092.0
81.90	501.0
86.90	1916.0
87.90	1952.0
91.00	251.0
91.90	1399.0
92.90	1978.0
93.90	5895.0
95.00	45272.0
95.90	3058.0
103.90	276.0
105.80	227.0
115.80	165.0
116.80	265.0
117.80	166.0
118.70	304.0
127.80	173.0
128.80	111.0
129.80	177.0
136.80	127.0
140.80	479.0
142.90	553.0
147.90	198.0
171.90	317.0
173.90	36104.0
174.90	2794.0
175.90	35744.0
176.90	2248.0

Instrument :
MSVOA_V
ClientSampleId :
BFB263

m/z	Abundance
39.70	253.0
40.00	201.0
43.80	151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB263

m/z	Abundance
35.80	473.0
36.90	2424.0
37.90	2215.0
38.90	820.0
39.80	287.0
43.80	498.0
45.00	444.0
46.80	581.0
47.90	360.0
48.90	2075.0
49.90	9337.0
50.90	3153.0
54.90	139.0
55.90	1023.0
56.90	1360.0
59.90	606.0
60.90	2528.0
61.90	2461.0
62.90	1857.0
64.00	309.0
64.90	337.0
67.00	135.0
67.90	4885.0
68.90	5474.0
69.90	454.0
71.80	269.0
72.90	2332.0
73.90	8770.0
74.90	24672.0
75.90	2232.0
77.00	375.0
77.80	108.0
78.80	1984.0
79.80	570.0
80.90	2149.0
81.90	557.0
86.90	2016.0
87.90	2061.0
91.00	247.0
91.90	1459.0
92.90	1943.0
93.90	6033.0
95.00	46816.0
95.90	3178.0
103.90	224.0
104.90	111.0
105.80	235.0
115.80	172.0
116.80	277.0
117.70	202.0
118.70	308.0
127.80	170.0
128.70	155.0
129.80	175.0
136.80	149.0
140.80	440.0
142.90	565.0
147.80	232.0
172.00	365.0
173.90	37880.0
174.90	2938.0
175.90	37080.0
176.90	2400.0

Instrument :
MSVOA_V
ClientSampleId :
BFB263

m/z	Abundance
35.80	395.0
36.90	2326.0
37.90	1955.0
38.90	797.0
39.80	283.0
43.80	484.0
45.00	454.0
46.80	499.0
47.90	327.0
48.90	1831.0
50.00	8512.0
50.90	2915.0
54.90	115.0
55.90	850.0
56.90	1199.0
59.90	595.0
60.90	2402.0
61.90	2238.0
62.90	1657.0
63.90	267.0
64.90	299.0
67.00	142.0
67.90	4628.0
68.90	5102.0
69.90	409.0
71.80	252.0
72.90	2132.0
73.90	8232.0
75.00	23232.0
75.90	2126.0
77.00	343.0
77.70	120.0
78.80	1850.0
79.80	626.0
80.90	2023.0
81.90	553.0
86.90	1920.0
87.90	1863.0
90.90	234.0
91.90	1428.0
92.90	1810.0
94.00	5582.0
95.00	43800.0
95.90	3012.0
103.90	210.0
104.90	131.0
105.80	221.0
115.80	174.0
116.70	325.0
117.70	256.0
118.70	279.0
127.70	159.0
128.70	171.0
129.80	170.0
136.80	160.0
140.80	427.0
142.80	591.0
144.90	113.0
147.70	240.0
149.90	102.0
156.90	107.0
172.00	337.0
173.90	35984.0
174.90	2802.0
175.90	35128.0
176.90	2379.0

Instrument :
MSVOA_V
ClientSampleId :
BFB263