

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV030220\
 Data File : VV014726.D
 Acq On : 02 Mar 2020 11:28
 Operator : SY/MD
 Sample : L1730-11
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Mar 03 01:01:22 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Mar 03 00:49:47 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	265636	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	253676	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	125358	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	96144	4.62	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.40%
7) Chloroethane-d5	1.58	69	79426	4.88	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.60%
11) 1,1-Dichloroethene-d2	2.13	63	124738	3.53	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.60%
20) 2-Butanone-d5	3.97	46	183460	42.68	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	85.36%
24) Chloroform-d	4.40	84	176559	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.60%
26) 1,2-Dichloroethane-d4	5.08	65	92089	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.60%
32) Benzene-d6	5.09	84	366584	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.60%
36) 1,2-Dichloropropane-d6	6.11	67	115730	5.03	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.60%
41) Toluene-d8	7.35	98	327281	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.20%
43) trans-1,3-Dichloropropene-	7.66	79	43068	4.84	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.80%
46) 2-Hexanone-d5	8.13	63	164748	45.76	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.52%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	79014	4.80	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	117170	5.03	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.60%


Target Compounds					Ovalue
16) Methylene chloride	2.53	84	4442	0.212 ug/L	98




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV030220\
Data File : VV014726.D
Acq On : 02 Mar 2020 11:28
Operator : SY/MD
Sample : L1730-11
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Mar 03 01:01:22 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Mar 03 00:49:47 2020
Response via : Initial Calibration

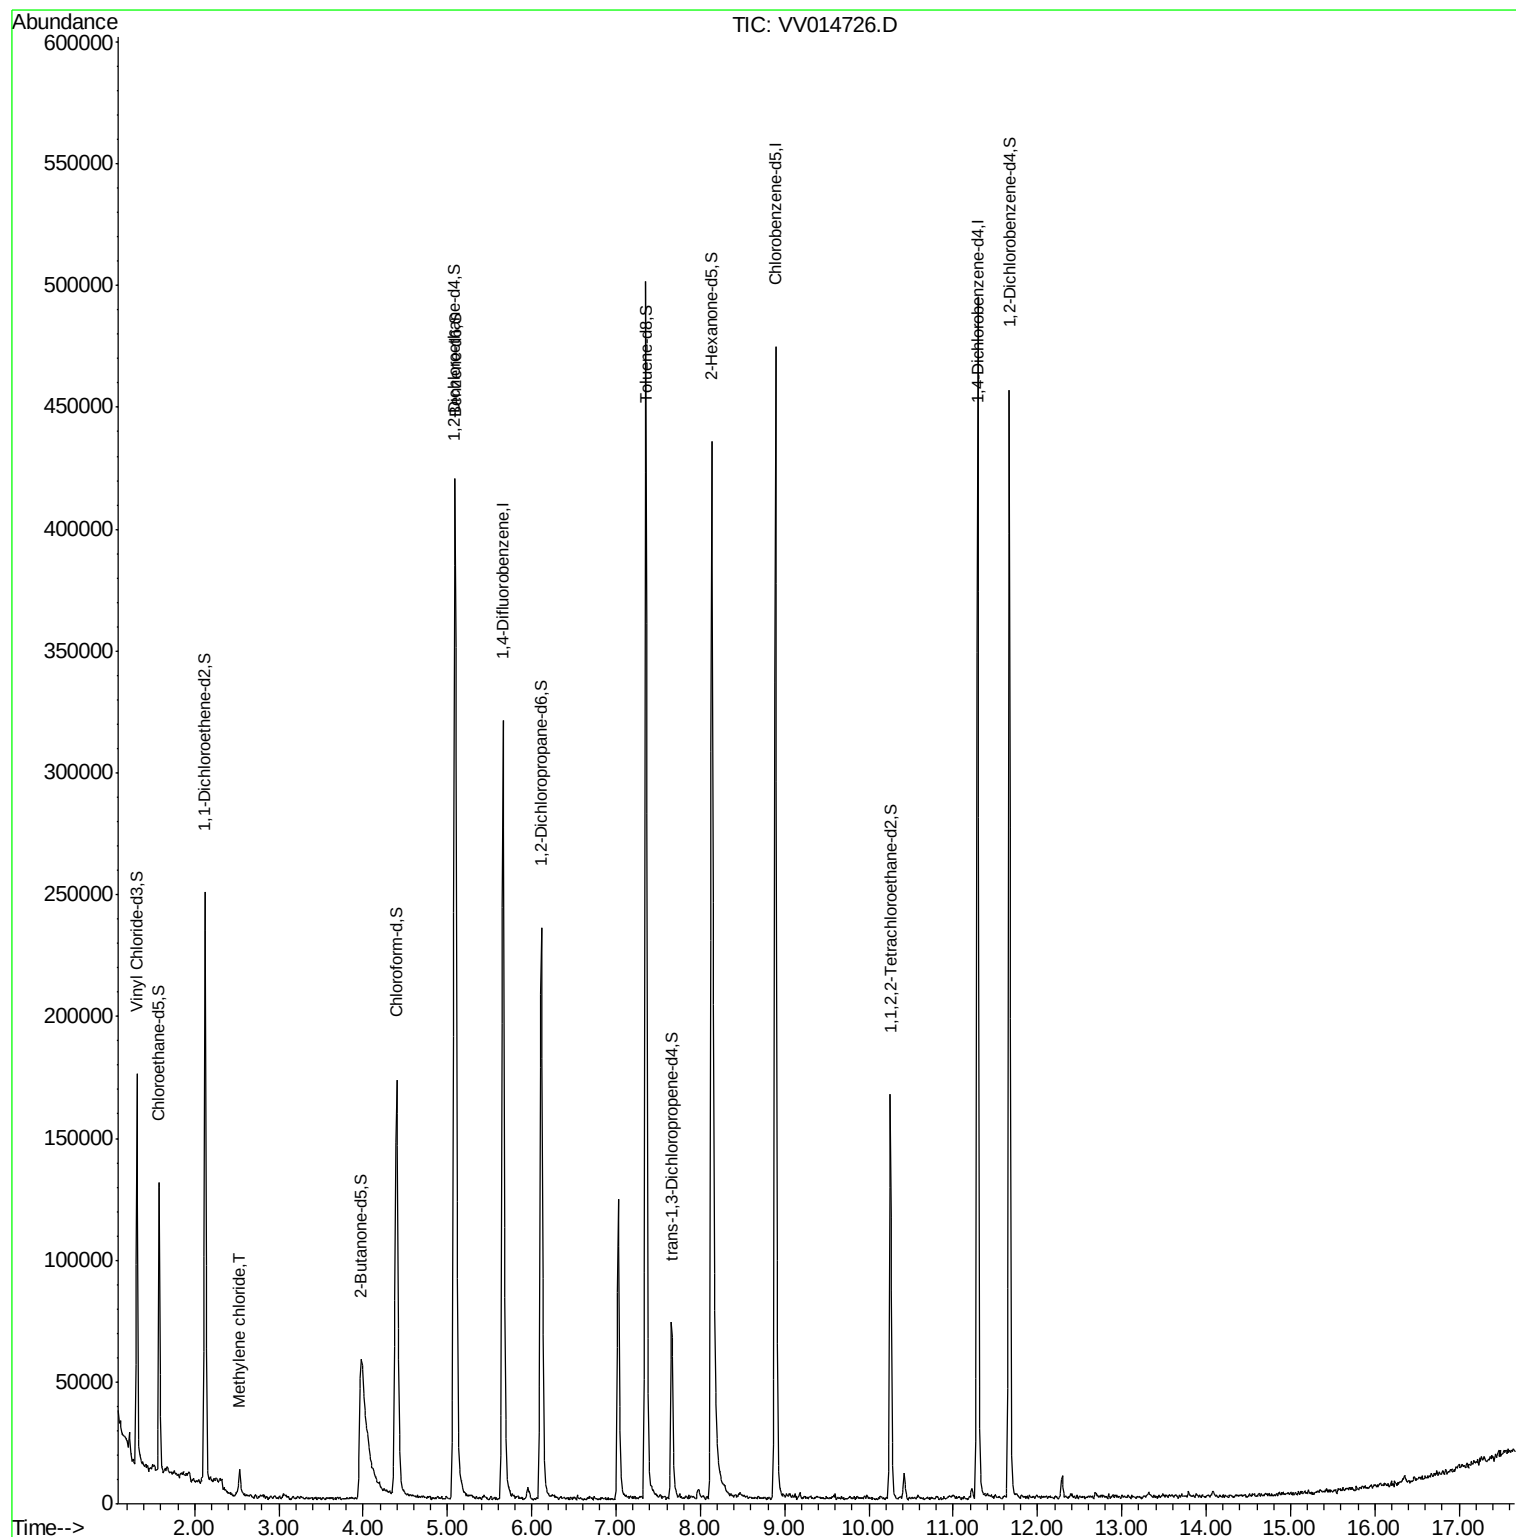

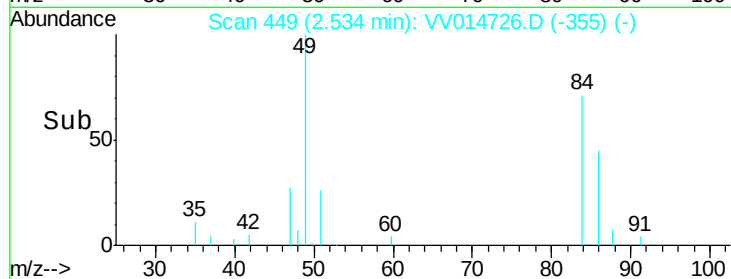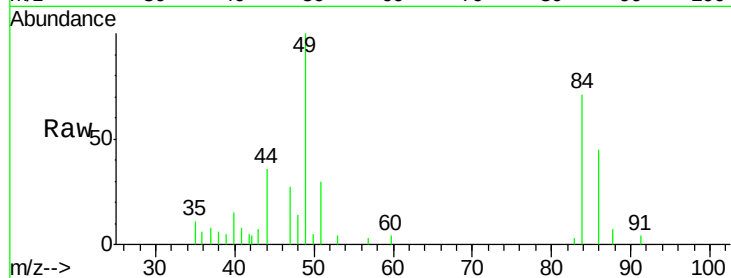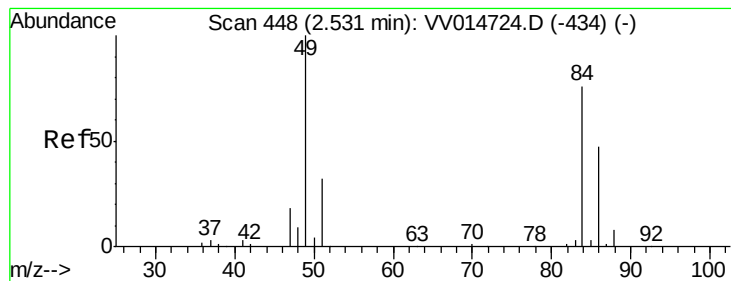

#16
 Methylene chloride
 Concen: 0.212 ug/L
 RT: 2.53 min Scan# 449
 Delta R.T. 0.00 min
 Lab File: VV014726.D
 Acq: 02 Mar 2020 11:28

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Tot Ion: 84 Resp: 4442
 Ion Ratio Lower Upper
 84 100
 86 63.8 44.9 83.5
 49 140.6 95.6 177.6

