


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV030220\
 Data File : VV014723.D
 Acq On : 02 Mar 2020 09:22
 Operator : SY/MD
 Sample : BFB40
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB40

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022820WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Mar 03 00:49:47 2020

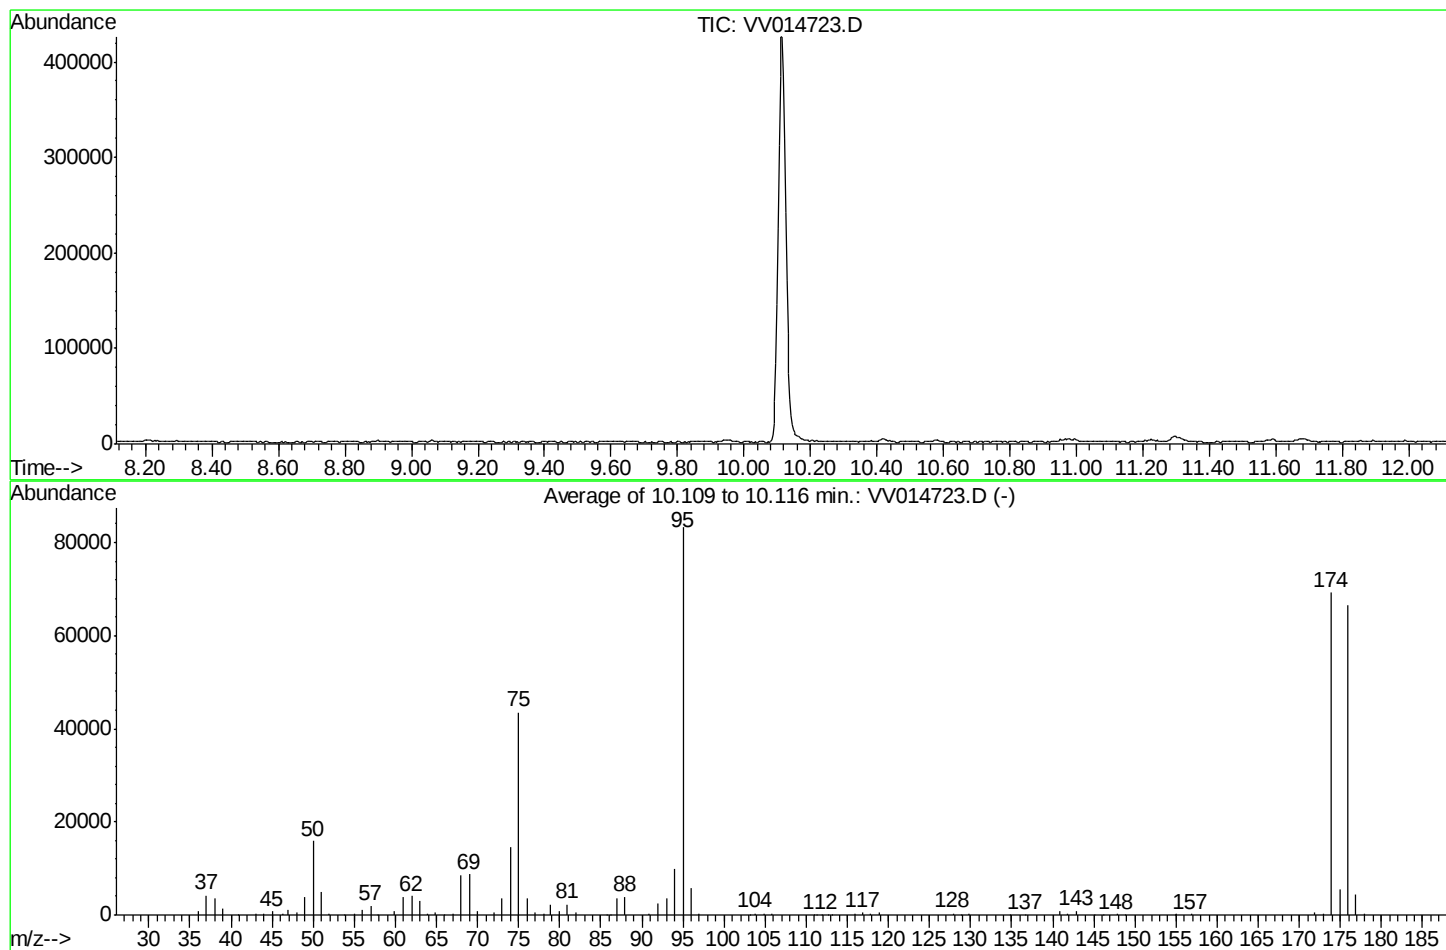

AutoFind: Scans 2805, 2806, 2807; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	15903	PASS
75	95	30	80	52.3	43538	PASS
95	95	100	100	100.0	83245	PASS
96	95	5	9	6.8	5696	PASS
173	174	0.00	2	0.4	250	PASS
174	95	50	120	83.1	69192	PASS
175	174	5	9	7.9	5446	PASS
176	174	95	101	96.0	66405	PASS
177	176	5	9	6.7	4481	PASS

m/z	Abundance
36.00	668.0
37.00	3988.0
38.00	3444.0
39.00	1335.0
39.90	527.0
43.00	133.0
44.00	1002.0
45.00	675.0
46.30	167.0
46.90	1008.0
48.00	478.0
49.00	3658.0
50.00	14855.0
51.00	4799.0
52.00	247.0
55.00	281.0
56.00	987.0
57.00	1888.0
59.90	835.0
61.00	3841.0
62.00	3873.0
63.00	2667.0
64.00	389.0
64.90	482.0
66.00	107.0
67.00	218.0
68.00	8121.0
69.00	8169.0
70.00	748.0
72.00	515.0
73.00	3312.0
74.00	13754.0
75.00	40688.0
76.00	3426.0
77.00	554.0
78.10	290.0
78.90	2034.0
79.90	746.0
80.90	2035.0
82.00	522.0
85.70	152.0
86.90	3363.0
87.90	3744.0
90.90	220.0
92.00	2345.0
93.00	3475.0
94.00	9290.0
95.00	78320.0
96.00	5402.0
96.90	153.0
103.80	384.0
104.90	134.0
105.80	356.0
110.90	173.0
111.90	104.0
113.20	106.0
115.80	278.0
116.90	418.0
117.90	289.0
118.90	435.0
127.90	261.0
129.00	151.0
129.80	324.0
134.90	163.0
136.70	110.0
140.90	812.0
141.90	143.0
142.90	908.0
145.00	132.0
147.90	203.0
148.80	117.0
154.80	222.0
156.90	167.0
171.90	343.0
172.90	752.0
173.90	63752.0
174.90	5245.0
175.90	60632.0
176.90	4017.0
177.90	168.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

m/z	Abundance
36.00	720.0
37.00	4414.0
38.00	3747.0
39.10	1502.0
39.90	588.0
43.00	157.0
44.00	1007.0
45.00	701.0
46.30	179.0
46.90	1153.0
48.00	602.0
49.00	3876.0
50.00	16326.0
51.00	5118.0
52.00	250.0
53.80	109.0
54.90	263.0
56.00	1148.0
57.00	1995.0
57.90	145.0
59.90	897.0
61.00	4047.0
62.00	4276.0
63.00	3008.0
64.00	407.0
64.90	503.0
66.00	150.0
67.10	223.0
68.00	8916.0
69.00	9021.0
70.00	802.0
72.00	565.0
73.00	3664.0
74.00	15002.0
75.00	45096.0
76.00	3728.0
77.00	518.0
78.00	364.0
78.90	2333.0
79.90	859.0
80.90	2328.0
82.00	605.0
85.70	107.0
86.20	188.0
86.90	3863.0
87.90	4087.0
90.90	261.0
92.00	2513.0
93.00	3574.0
94.00	10040.0
95.00	85808.0
96.00	5876.0
96.90	168.0
103.20	117.0
103.80	434.0
104.80	157.0
105.80	375.0
110.90	126.0
111.80	122.0
115.90	312.0
116.90	554.0
117.90	366.0
118.90	428.0
127.80	293.0
128.90	130.0
129.80	275.0
134.80	130.0
136.70	142.0
140.90	868.0
141.80	159.0
143.00	980.0
145.10	106.0
146.10	106.0
147.90	217.0
155.00	251.0
156.90	231.0
171.90	415.0
173.90	71440.0
174.90	5645.0
175.90	68664.0
176.90	4627.0
177.90	153.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

m/z	Abundance
36.10	732.0
37.00	4221.0
38.00	3694.0
39.00	1482.0
39.90	598.0
40.90	144.0
42.90	179.0
44.00	975.0
45.00	715.0
46.20	167.0
46.90	1190.0
48.00	646.0
49.00	3742.0
50.00	16528.0
51.00	4986.0
51.90	204.0
54.90	230.0
56.00	1141.0
57.00	2016.0
57.90	169.0
59.90	841.0
61.00	3859.0
62.00	4148.0
63.00	3077.0
63.90	321.0
64.90	469.0
66.00	145.0
67.10	256.0
68.00	8787.0
69.00	9134.0
70.00	806.0
72.00	549.0
73.00	3732.0
74.00	14762.0
75.00	44832.0
76.00	3662.0
77.00	525.0
78.00	402.0
78.90	2435.0
79.90	777.0
80.90	2349.0
81.90	654.0
86.20	199.0
86.90	3817.0
88.00	4015.0
90.80	289.0
92.00	2493.0
93.00	3471.0
94.00	10030.0
95.00	85608.0
96.00	5811.0
97.00	166.0
103.80	451.0
104.90	166.0
105.90	336.0
111.30	117.0
111.80	110.0
112.60	112.0
115.90	302.0
116.90	598.0
117.80	384.0
118.80	411.0
127.80	319.0
128.80	102.0
129.80	215.0
134.80	131.0
136.70	182.0
140.90	855.0
141.80	151.0
143.00	1017.0
147.80	201.0
155.10	306.0
156.90	247.0
171.90	529.0
173.90	72384.0
174.90	5448.0
175.90	69920.0
176.90	4801.0
177.90	143.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

Scan 2793 (10.071 min): VV014723.D
BFB40

m/z	Abundance
39.90	609.0
41.80	123.0
44.00	749.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40