

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW030221\
 Data File : VW020428.D
 Acq On : 02 Mar 2021 10:20
 Operator : SY/MD
 Sample : VSTD0.0536
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.05302

Quant Time: Mar 03 00:24:16 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030221.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Mar 03 00:23:40 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc Units	Dev(Min)
Internal Standards					
1) 1,4-Difluorobenzene	5.639	114	13566	0.50 ug/L	0.00
5) Chlorobenzene-d5	8.864	117	12657	0.50 ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	6473	0.50 ug/L	0.00
System Monitoring Compounds					
2) Vinyl Chloride-d3	1.310	65	708	0.04 ug/L	0.00
4) 1,2-Dichloroethane-d4	5.043	65	391	0.04 ug/L	0.00
7) 1,2-Dichloropropane-d6	6.069	67	468	0.04 ug/L	0.00
8) Toluene-d8	7.332	98	1466	0.05 ug/L	0.02
10) 1,1,2,2-Tetrachloroeth...	10.216	84	266	0.04 ug/L	0.00
Target Compounds					
3) Vinyl chloride	1.310	62	839	0.05 ug/L	Qvalue 85
6) Trichloroethene	5.925	95	566	0.06 ug/L	93
9) 1,2-Dibromoethane	8.369	107	297	0.05 ug/L #	92
12) 1,2,3-Trichloropropane	10.267	75	281	0.05 ug/L	99
13) 1,2-Dibromo-3-chloropr...	12.427	75	44	0.05 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030221\
Data File : VV020428.D
Acq On : 02 Mar 2021 10:20
Operator : SY/MD
Sample : VSTD0.0536
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.05302

Quant Time: Mar 03 00:24:16 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030221.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Mar 03 00:23:40 2021
Response via : Initial Calibration




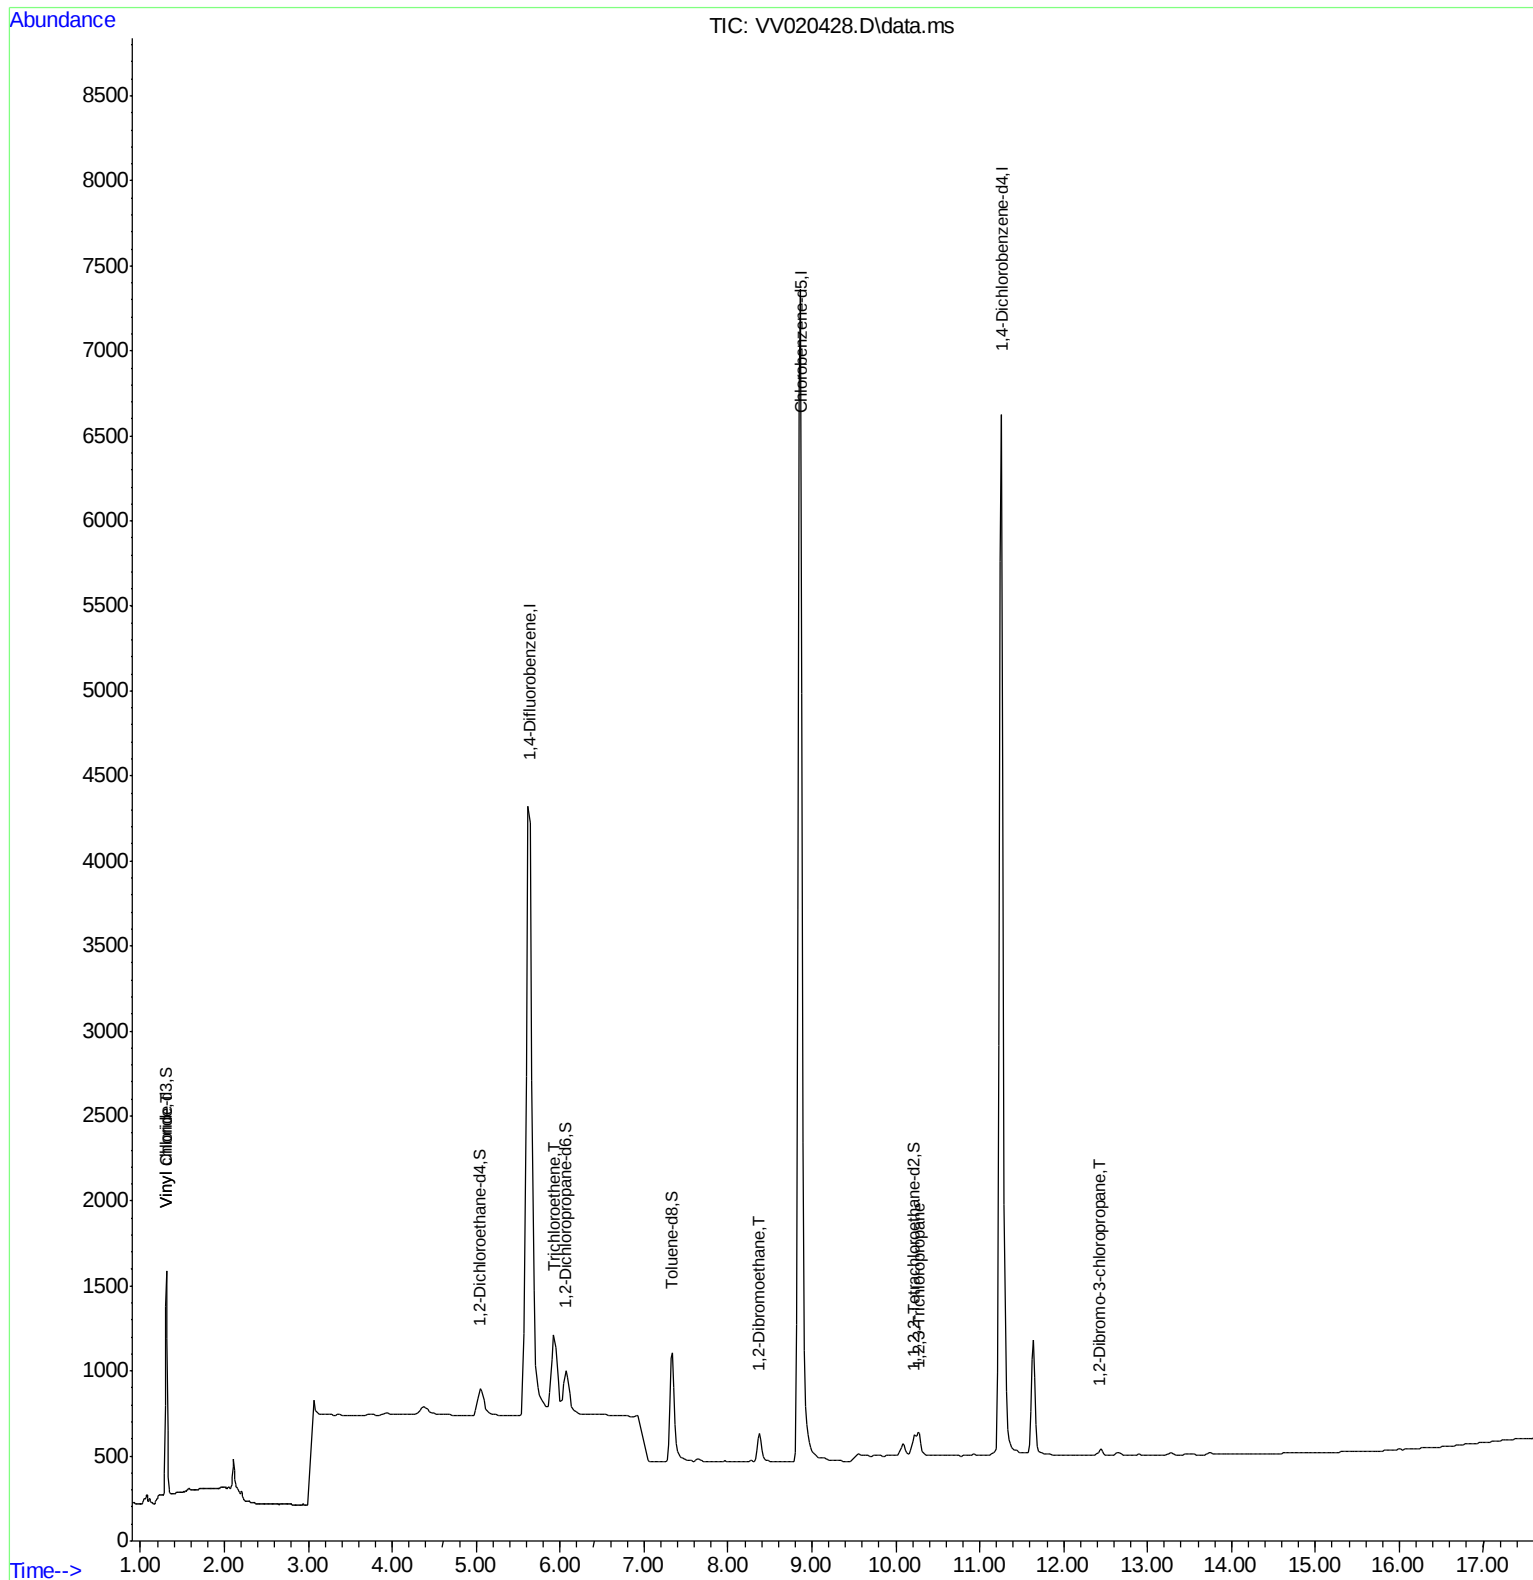


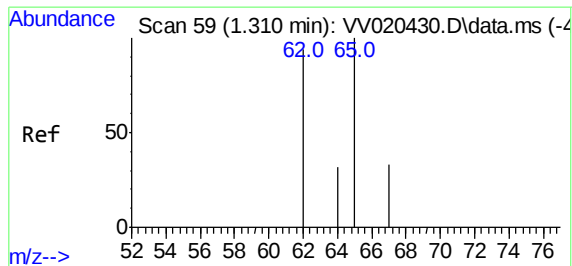

#3
 Vinyl chloride
 Concen: 0.05 ug/L
 RT: 1.310 min Scan# 59
 Delta R.T. 0.000 min
 Lab File: VV020428.D
 Acq: 02 Mar 2021 10:20




Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.05302


Tgt Ion: 62 Resp: 839
 Ion Ratio Lower Upper
 62 100
 64 43.1 24.3 45.1

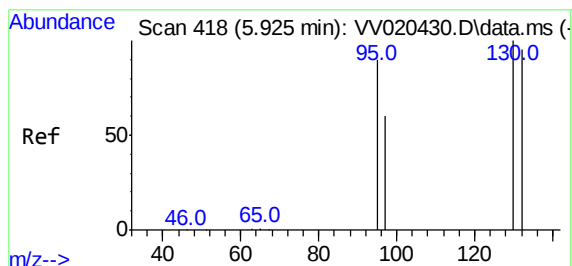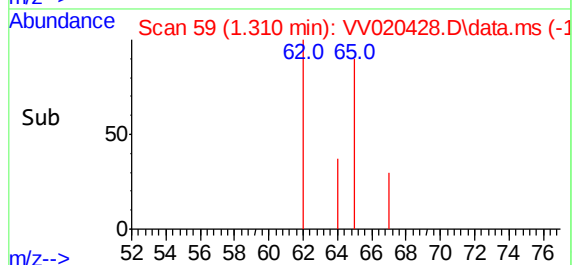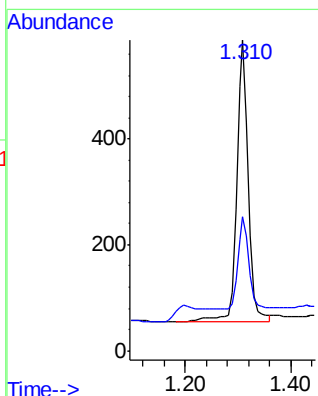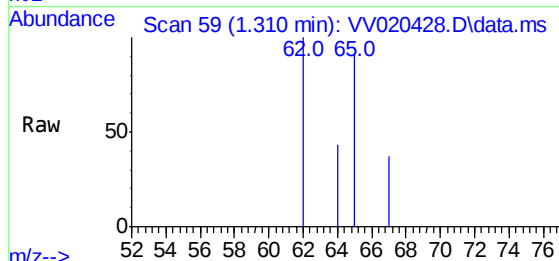

#6
 Trichloroethene
 Concen: 0.06 ug/L
 RT: 5.925 min Scan# 418
 Delta R.T. 0.000 min
 Lab File: VV020428.D
 Acq: 02 Mar 2021 10:20

Tgt Ion: 95 Resp: 566
 Ion Ratio Lower Upper
 95 100
 97 75.9 47.2 87.6
 132 98.2 73.6 136.6
 130 104.1 77.1 143.3


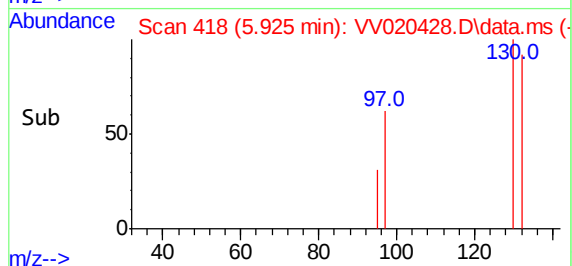
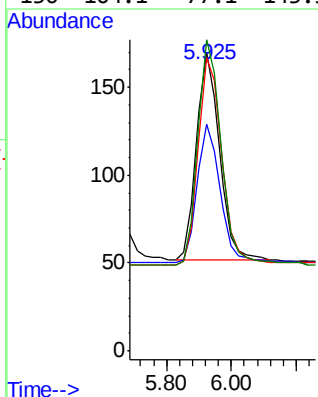
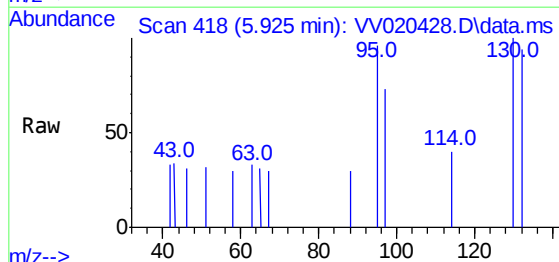


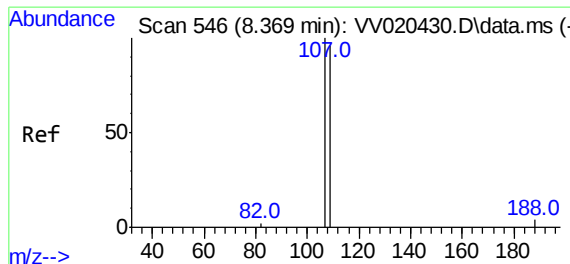

#9
1,2-Dibromoethane
Concen: 0.05 ug/L
RT: 8.369 min Scan# 546
Delta R.T. 0.000 min
Lab File: VV020428.D
Acq: 02 Mar 2021 10:20




Instrument :
MSVOA_V
ClientSampleId :
VSTD0.05302


Tgt Ion:107 Resp: 297
Ion Ratio Lower Upper
107 100
109 97.0 67.3 125.1
188 38.6 7.8 11.8#

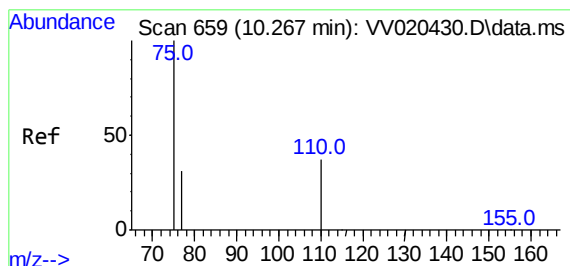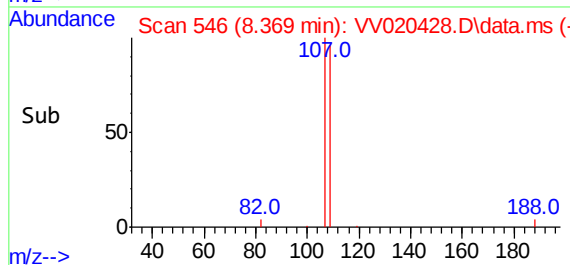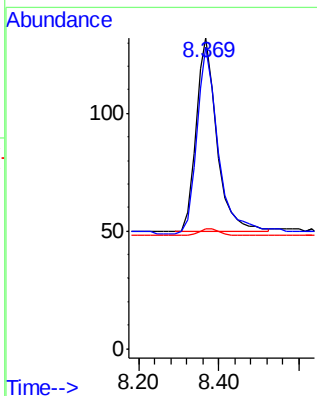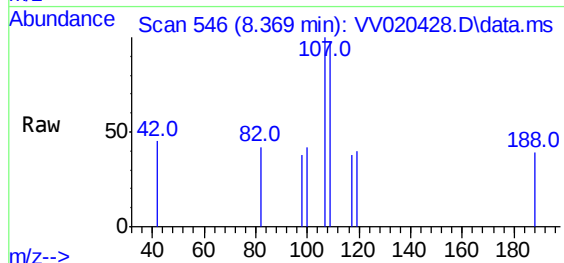

#12
1,2,3-Trichloropropane
Concen: 0.05 ug/L
RT: 10.267 min Scan# 659
Delta R.T. 0.000 min
Lab File: VV020428.D
Acq: 02 Mar 2021 10:20


Tgt Ion: 75 Resp: 281
Ion Ratio Lower Upper
75 100
110 41.6 33.5 50.3
77 33.1 25.4 38.2

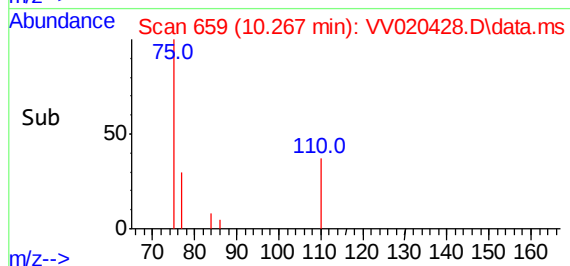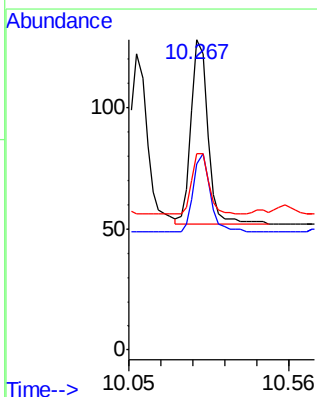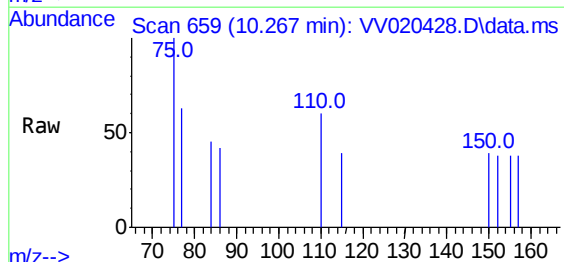

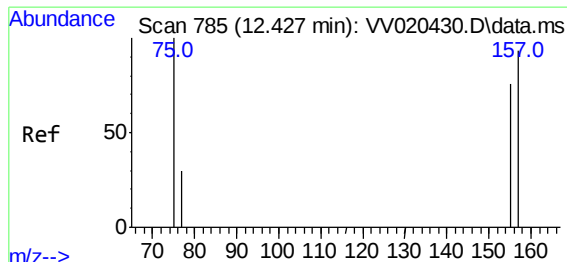

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.05 ug/L
 RT: 12.427 min Scan# 785
 Delta R.T. 0.000 min
 Lab File: VV020428.D
 Acq: 02 Mar 2021 10:20

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.05302

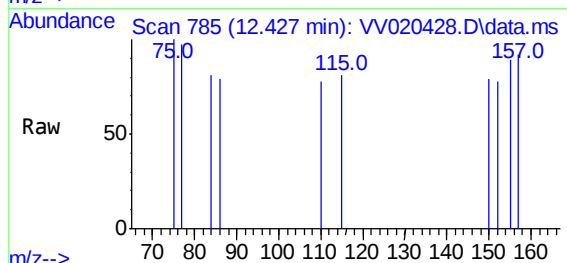

Tgt Ion: 75 Resp: 44
 Ion Ratio Lower Upper
 75 100
 157 92.1 74.3 111.5
 155 88.9 65.4 98.2

