

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW030221\
 Data File : VW020429.D
 Acq On : 02 Mar 2021 11:07
 Operator : SY/MD
 Sample : VSTD0.131
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.1303

Quant Time: Mar 03 00:24:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030221.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Mar 03 00:23:40 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc Units	Dev(Min)
Internal Standards					
1) 1,4-Difluorobenzene	5.639	114	12321	0.50 ug/L	0.00
5) Chlorobenzene-d5	8.863	117	12077	0.50 ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	6088	0.50 ug/L	0.00
System Monitoring Compounds					
2) Vinyl Chloride-d3	1.310	65	1370	0.09 ug/L	0.00
4) 1,2-Dichloroethane-d4	5.042	65	792	0.09 ug/L	0.00
7) 1,2-Dichloropropane-d6	6.068	67	926	0.08 ug/L	0.00
8) Toluene-d8	7.332	98	2799	0.09 ug/L	0.02
10) 1,1,2,2-Tetrachloroeth...	10.216	84	505	0.08 ug/L	0.00
Target Compounds					
3) Vinyl chloride	1.310	62	1434	0.10 ug/L	Qvalue 92
6) Trichloroethene	5.925	95	984	0.10 ug/L	94
9) 1,2-Dibromoethane	8.368	107	562	0.10 ug/L #	96
12) 1,2,3-Trichloropropane	10.267	75	503	0.10 ug/L	98
13) 1,2-Dibromo-3-chloropr...	12.426	75	69	0.08 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030221\
Data File : VV020429.D
Acq On : 02 Mar 2021 11:07
Operator : SY/MD
Sample : VSTD0.131
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.1303

Quant Time: Mar 03 00:24:26 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030221.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Mar 03 00:23:40 2021
Response via : Initial Calibration

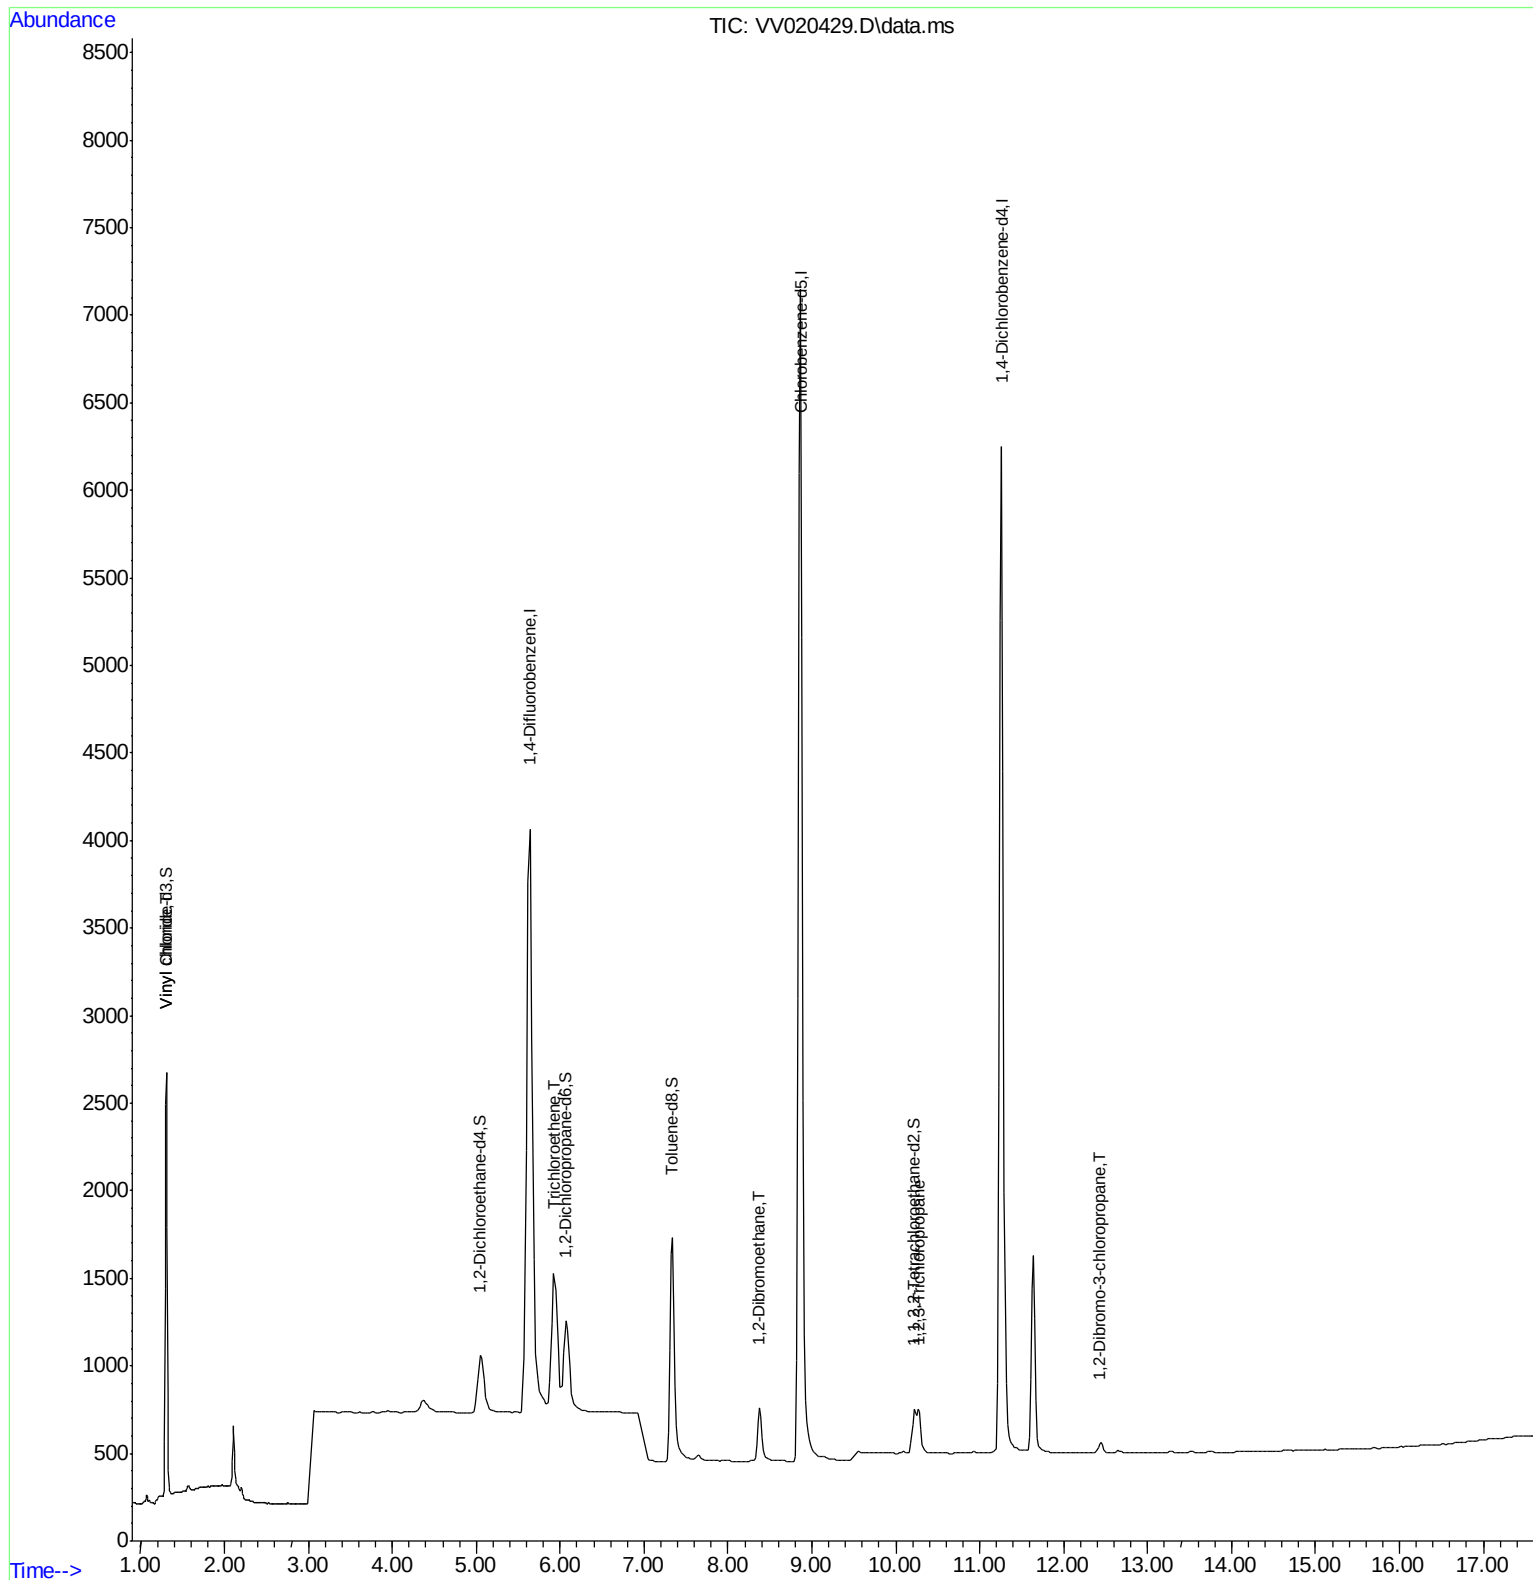




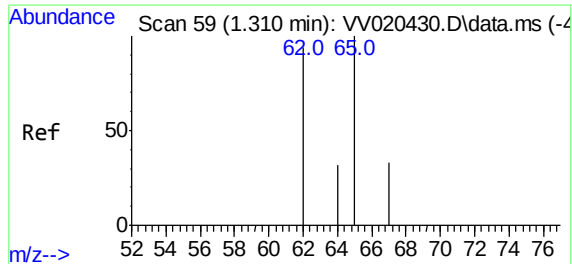


#3

Vinyl chloride
Concen: 0.10 ug/L
RT: 1.310 min Scan# 59
Delta R.T. -0.000 min
Lab File: VV020429.D
Acq: 02 Mar 2021 11:07

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.1303




Tgt Ion: 62 Resp: 1434
Ion Ratio Lower Upper
62 100
64 39.2 24.3 45.1

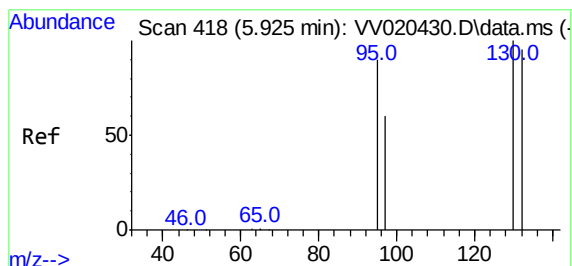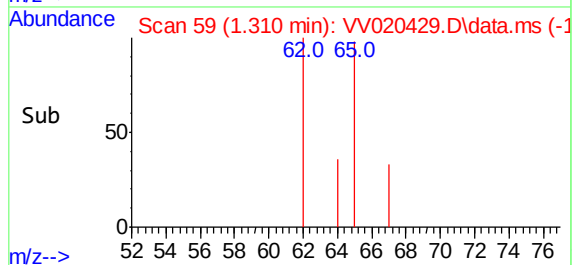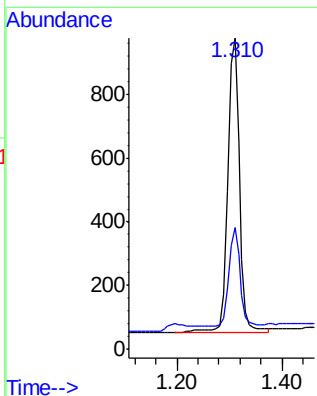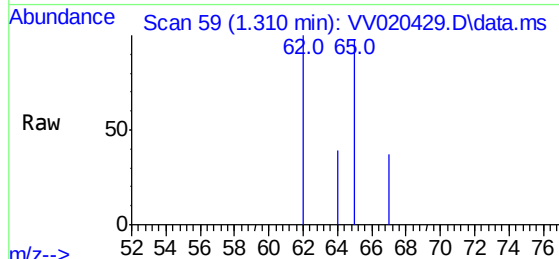


#6

Trichloroethene
Concen: 0.10 ug/L
RT: 5.925 min Scan# 418
Delta R.T. -0.000 min
Lab File: VV020429.D
Acq: 02 Mar 2021 11:07

Tgt Ion: 95 Resp: 984
Ion Ratio Lower Upper
95 100
97 70.7 47.2 87.6
132 97.7 73.6 136.6
130 102.7 77.1 143.3


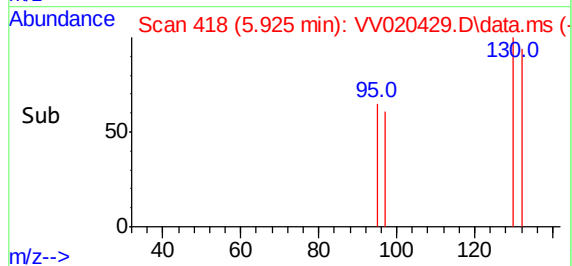
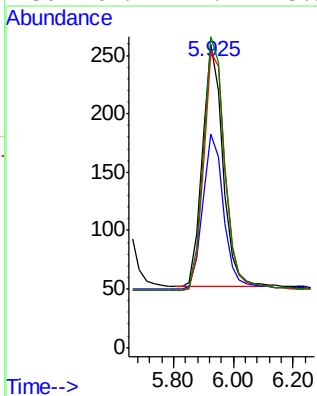
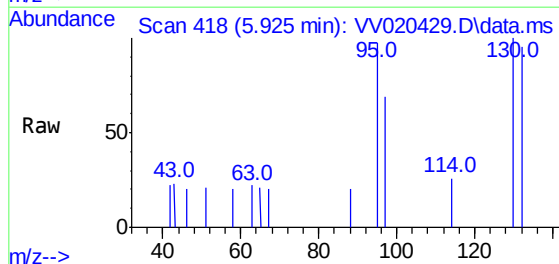


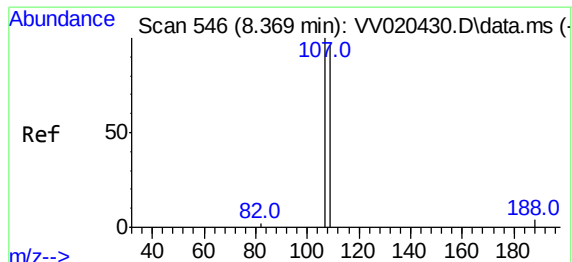

#9
1,2-Dibromoethane
Concen: 0.10 ug/L
RT: 8.368 min Scan# 546
Delta R.T. -0.000 min
Lab File: VV020429.D
Acq: 02 Mar 2021 11:07




Instrument :
MSVOA_V
ClientSampleId :
VSTD0.1303


Tgt Ion:107 Resp: 562
Ion Ratio Lower Upper
107 100
109 96.0 67.3 125.1
188 27.0 7.8 11.8#

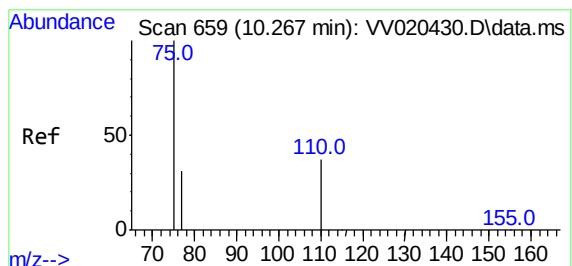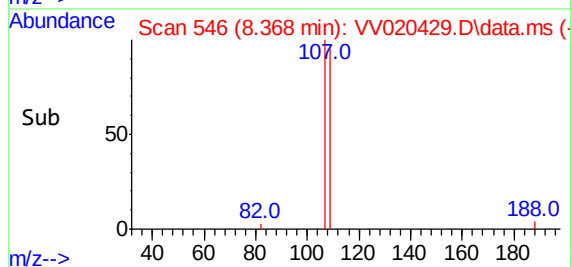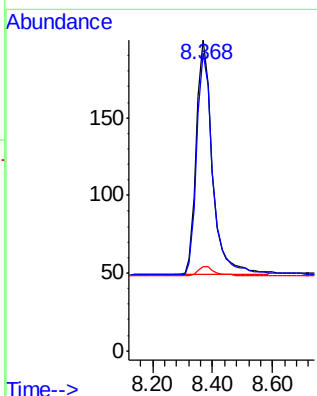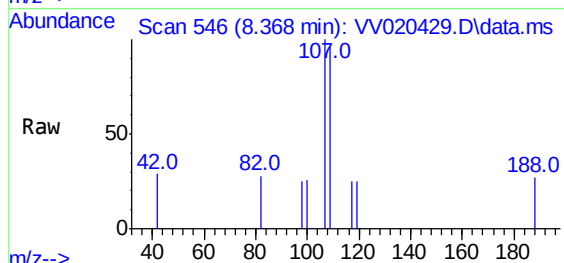

#12
1,2,3-Trichloropropane
Concen: 0.10 ug/L
RT: 10.267 min Scan# 659
Delta R.T. -0.000 min
Lab File: VV020429.D
Acq: 02 Mar 2021 11:07


Tgt Ion: 75 Resp: 503
Ion Ratio Lower Upper
75 100
110 42.7 33.5 50.3
77 33.6 25.4 38.2

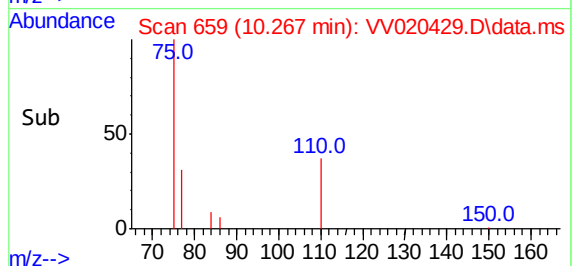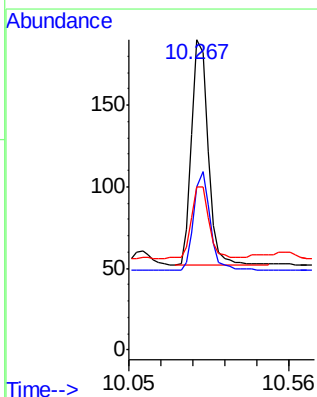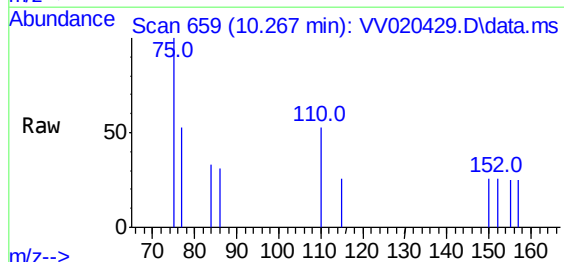

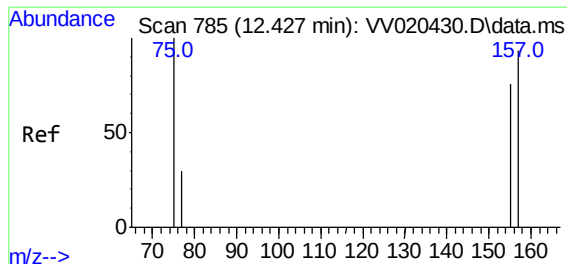

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.08 ug/L
 RT: 12.426 min Scan# 785
 Delta R.T. -0.000 min
 Lab File: VV020429.D
 Acq: 02 Mar 2021 11:07

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.1303

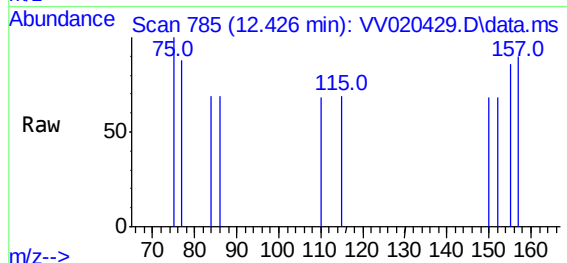

Tgt Ion: 75 Resp: 69
 Ion Ratio Lower Upper
 75 100
 157 90.3 74.3 111.5
 155 86.1 65.4 98.2

