

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW030221\
 Data File : VW020430.D
 Acq On : 02 Mar 2021 11:30
 Operator : SY/MD
 Sample : VSTD0.532
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5304

Quant Time: Mar 03 00:24:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030221.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Mar 03 00:23:40 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc Units	Dev(Min)
Internal Standards					
1) 1,4-Difluorobenzene	5.639	114	12741	0.50 ug/L	0.00
5) Chlorobenzene-d5	8.864	117	12464	0.50 ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	6229	0.50 ug/L	0.00
System Monitoring Compounds					
2) Vinyl Chloride-d3	1.310	65	7668	0.48 ug/L	0.00
4) 1,2-Dichloroethane-d4	5.042	65	4371	0.46 ug/L	0.00
7) 1,2-Dichloropropane-d6	6.068	67	5490	0.48 ug/L	0.00
8) Toluene-d8	7.317	98	15550	0.49 ug/L	0.00
10) 1,1,2,2-Tetrachloroeth...	10.216	84	2810	0.42 ug/L	0.00
Target Compounds					
3) Vinyl chloride	1.310	62	7083	0.49 ug/L	Qvalue 100
6) Trichloroethene	5.925	95	4932	0.49 ug/L	100
9) 1,2-Dibromoethane	8.369	107	2839	0.49 ug/L	100
12) 1,2,3-Trichloropropane	10.267	75	2558	0.49 ug/L	100
13) 1,2-Dibromo-3-chloropr...	12.427	75	339	0.38 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030221\
Data File : VV020430.D
Acq On : 02 Mar 2021 11:30
Operator : SY/MD
Sample : VSTD0.532
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5304

Quant Time: Mar 03 00:24:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030221.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Mar 03 00:23:40 2021
Response via : Initial Calibration




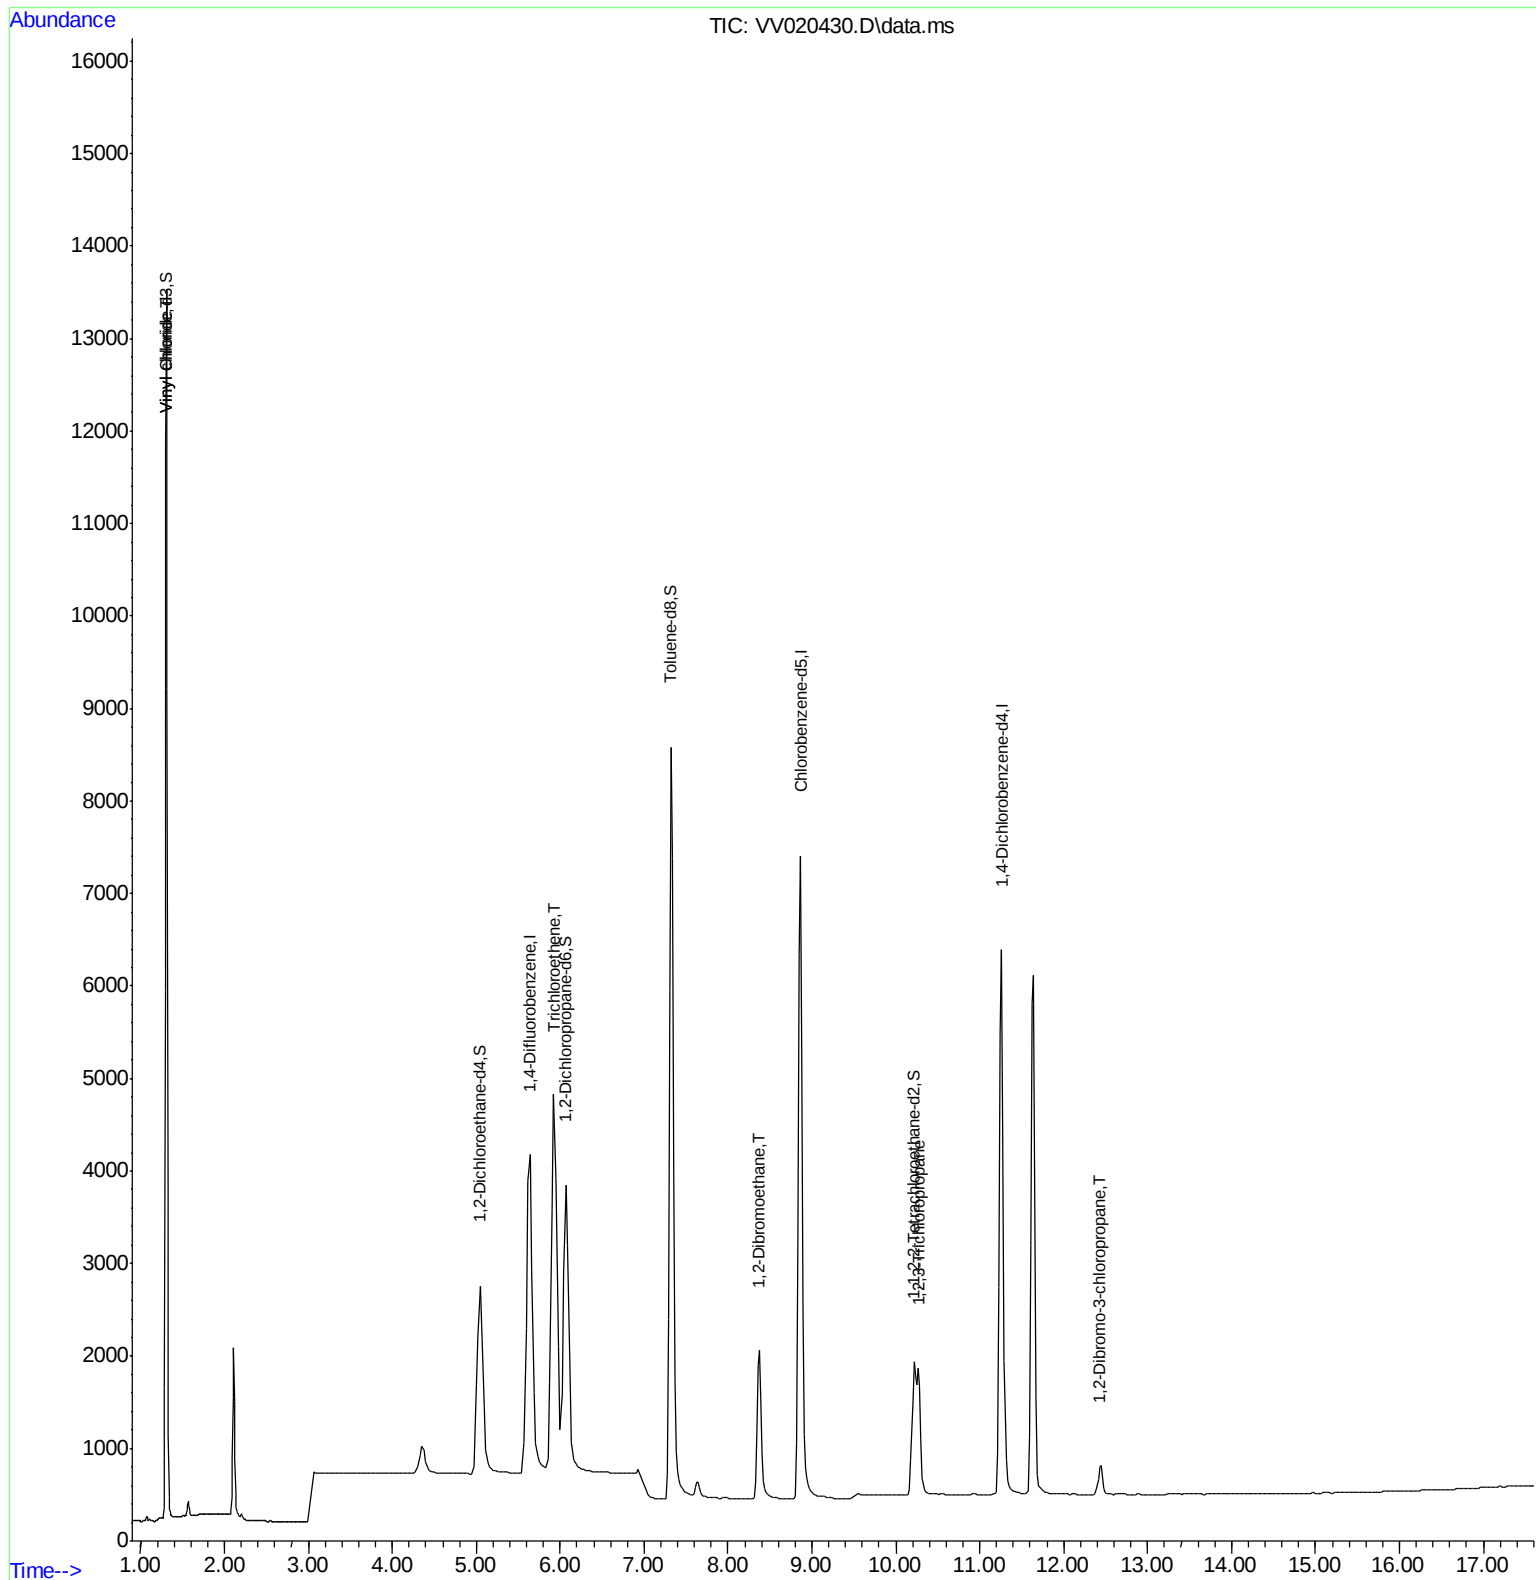


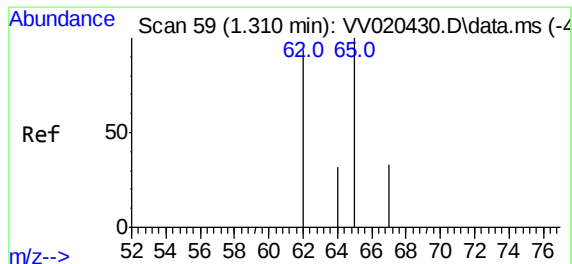

#3
 Vinyl chloride
 Concen: 0.49 ug/L
 RT: 1.310 min Scan# 59
 Delta R.T. 0.000 min
 Lab File: VV020430.D
 Acq: 02 Mar 2021 11:30




Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5304


Tgt Ion: 62 Resp: 7083
 Ion Ratio Lower Upper
 62 100
 64 34.7 24.3 45.1

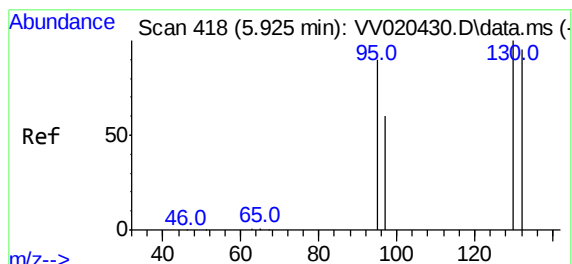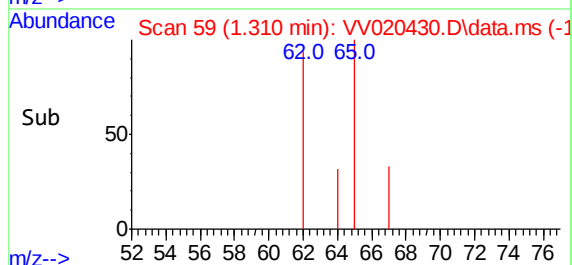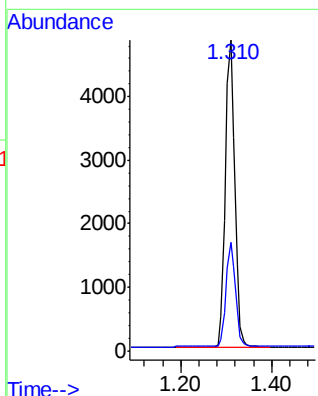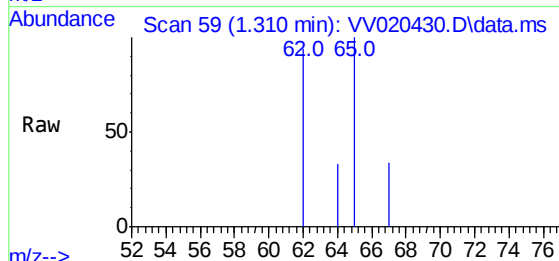

#6
 Trichloroethene
 Concen: 0.49 ug/L
 RT: 5.925 min Scan# 418
 Delta R.T. 0.000 min
 Lab File: VV020430.D
 Acq: 02 Mar 2021 11:30

Tgt Ion: 95 Resp: 4932
 Ion Ratio Lower Upper
 95 100
 97 67.4 47.2 87.6
 132 105.1 73.6 136.6
 130 110.2 77.1 143.3


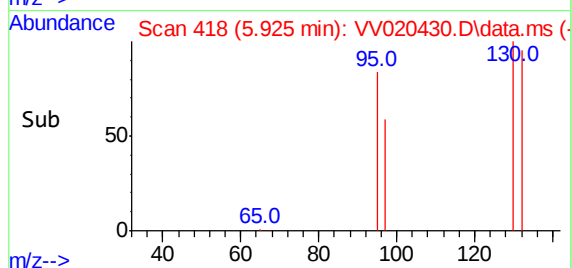
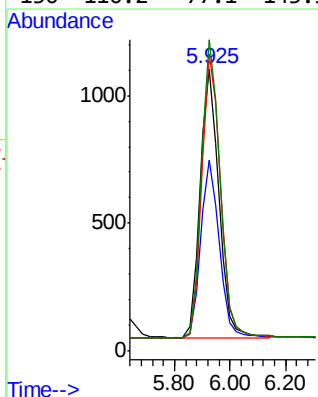
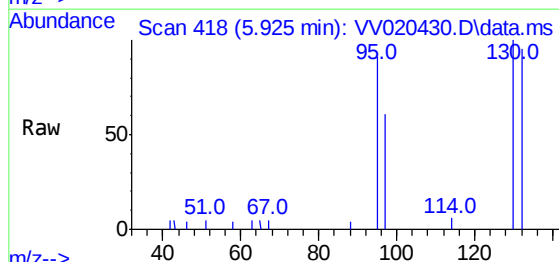


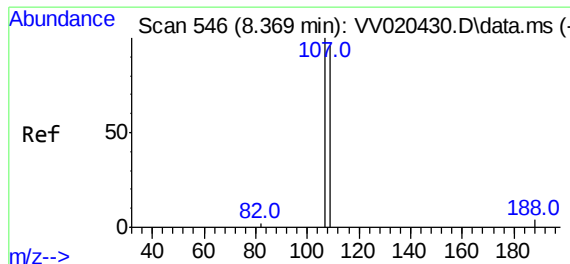

#9
1,2-Dibromoethane
Concen: 0.49 ug/L
RT: 8.369 min Scan# 546
Delta R.T. 0.000 min
Lab File: VV020430.D
Acq: 02 Mar 2021 11:30




Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5304


Tgt Ion:107 Resp: 2839
Ion Ratio Lower Upper
107 100
109 96.2 67.3 125.1
188 9.8 7.8 11.8

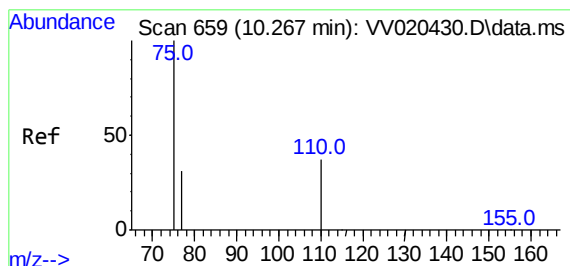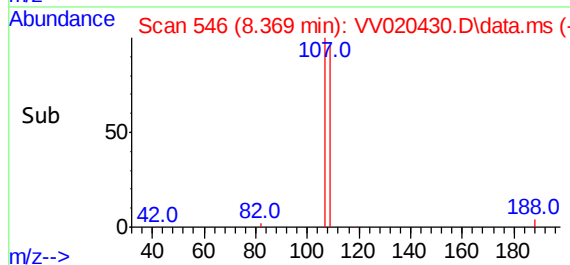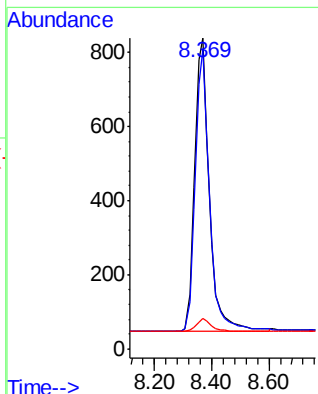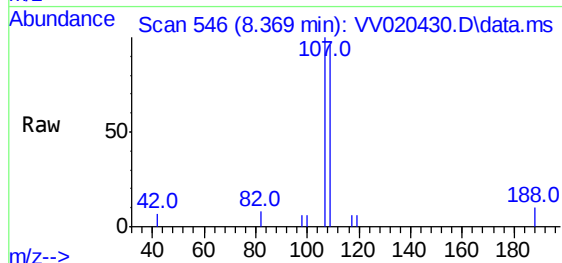

#12
1,2,3-Trichloropropane
Concen: 0.49 ug/L
RT: 10.267 min Scan# 659
Delta R.T. 0.000 min
Lab File: VV020430.D
Acq: 02 Mar 2021 11:30


Tgt Ion: 75 Resp: 2558
Ion Ratio Lower Upper
75 100
110 41.9 33.5 50.3
77 31.7 25.4 38.2

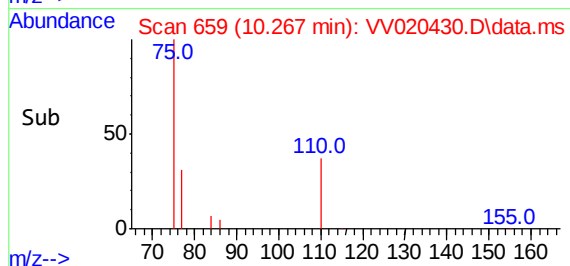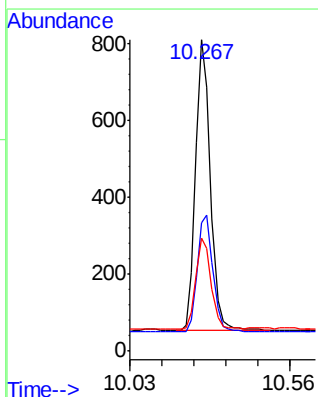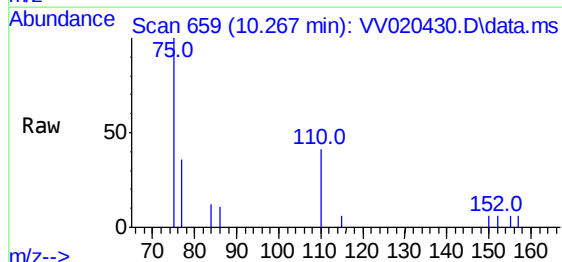

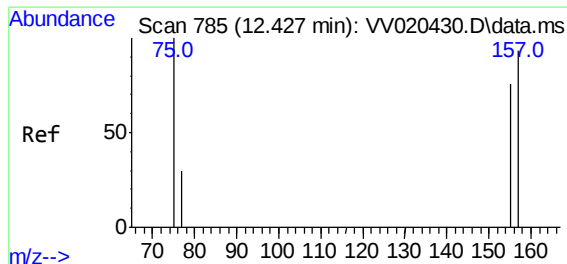

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.38 ug/L
 RT: 12.427 min Scan# 785
 Delta R.T. 0.000 min
 Lab File: VV020430.D
 Acq: 02 Mar 2021 11:30

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5304

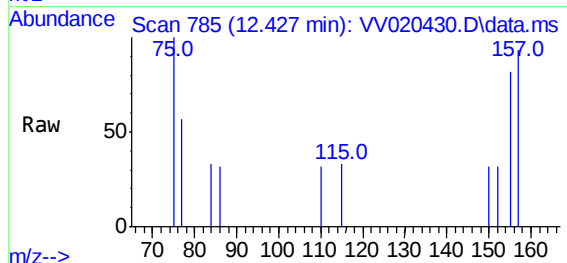

Tgt Ion: 75 Resp: 339
 Ion Ratio Lower Upper
 75 100
 157 92.9 74.3 111.5
 155 81.8 65.4 98.2

