

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW030221\
 Data File : VW020432.D
 Acq On : 02 Mar 2021 12:20
 Operator : SY/MD
 Sample : VSTD00234
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD002306

Quant Time: Mar 03 00:24:57 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030221.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Mar 03 00:23:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)


Internal Standards					
1) 1,4-Difluorobenzene	5.639	114	12822	0.50 ug/L	0.00
5) Chlorobenzene-d5	8.864	117	12582	0.50 ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	6345	0.50 ug/L	0.00
System Monitoring Compounds					
2) Vinyl Chloride-d3	1.303	65	30626	1.90 ug/L	0.00
4) 1,2-Dichloroethane-d4	5.042	65	18098	1.88 ug/L	0.00
7) 1,2-Dichloropropane-d6	6.069	67	21796	1.90 ug/L	0.00
8) Toluene-d8	7.317	98	66237	2.05 ug/L	0.00
10) 1,1,2,2-Tetrachloroeth...	10.216	84	11380	1.70 ug/L	0.00
Target Compounds					
					Qvalue
3) Vinyl chloride	1.310	62	28151	1.95 ug/L	100
6) Trichloroethene	5.925	95	20371	2.01 ug/L	99
9) 1,2-Dibromoethane	8.353	107	11762	2.00 ug/L #	95
12) 1,2,3-Trichloropropane	10.267	75	10403	1.94 ug/L	100
13) 1,2-Dibromo-3-chloropr...	12.427	75	1337	1.48 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030221\
Data File : VV020432.D
Acq On : 02 Mar 2021 12:20
Operator : SY/MD
Sample : VSTD00234
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD002306

Quant Time: Mar 03 00:24:57 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030221.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Mar 03 00:23:40 2021
Response via : Initial Calibration




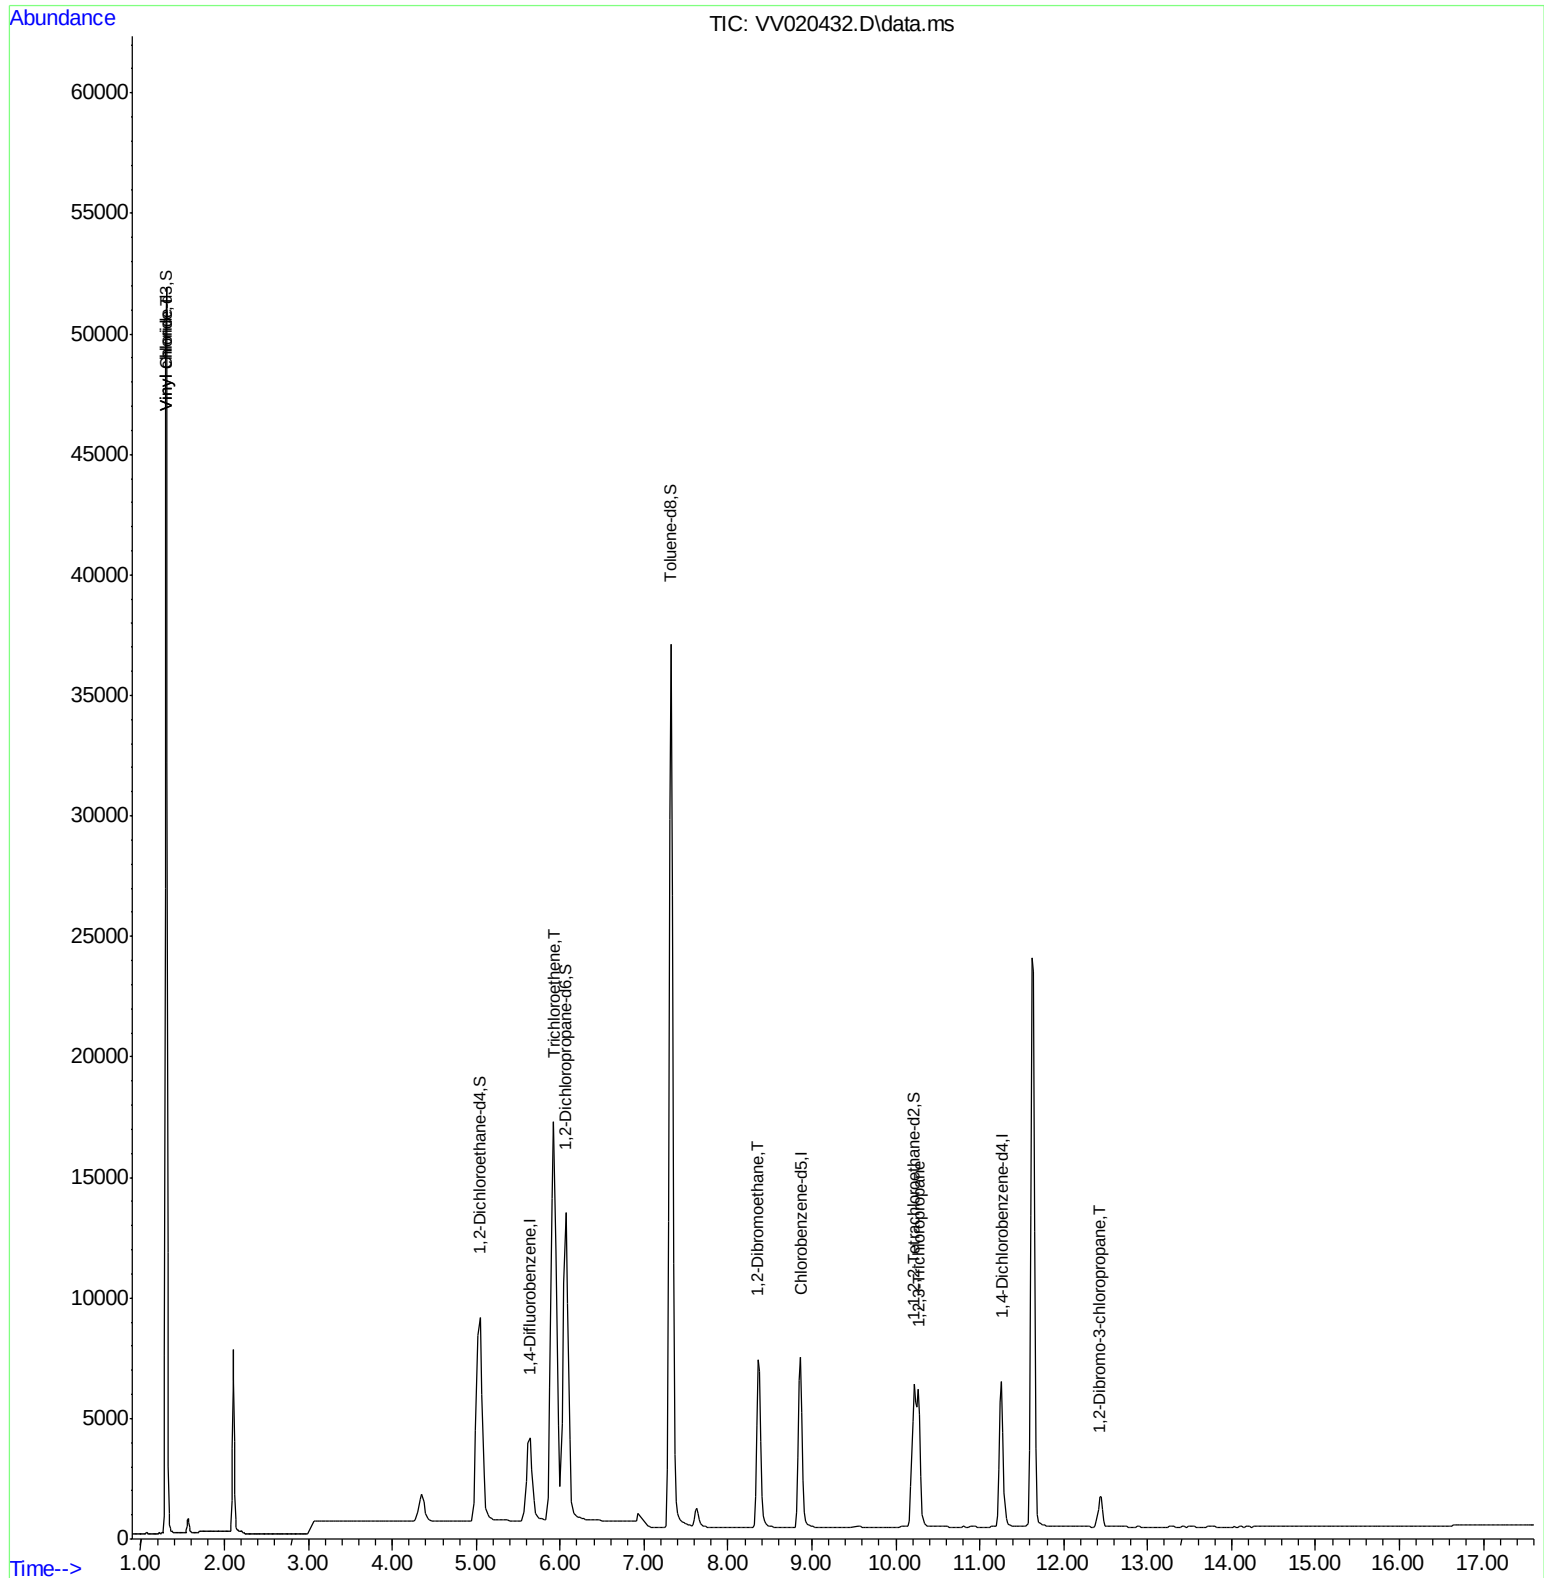


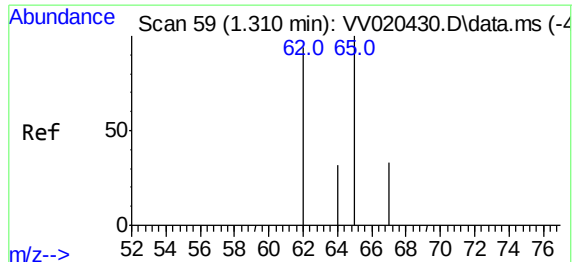

#3
Vinyl chloride
Concen: 1.95 ug/L
RT: 1.310 min Scan# 59
Delta R.T. 0.000 min
Lab File: VV020432.D
Acq: 02 Mar 2021 12:20




Instrument :
MSVOA_V
ClientSampleId :
VSTD002306


Tgt Ion: 62 Resp: 28151
Ion Ratio Lower Upper
62 100
64 34.5 24.3 45.1

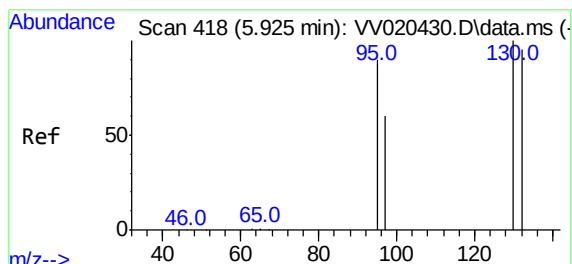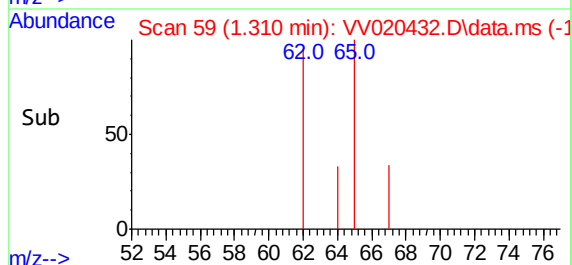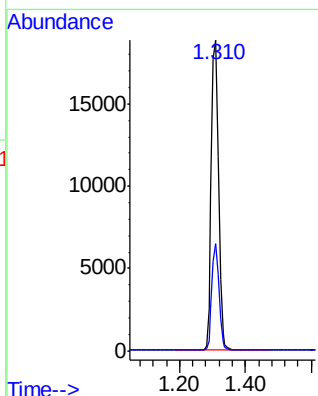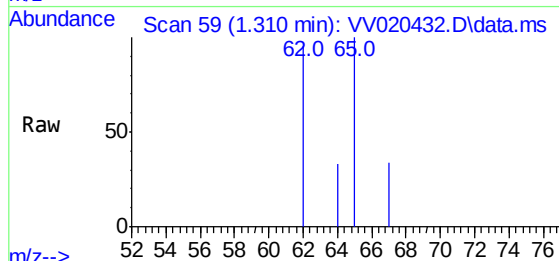

#6
Trichloroethene
Concen: 2.01 ug/L
RT: 5.925 min Scan# 418
Delta R.T. 0.000 min
Lab File: VV020432.D
Acq: 02 Mar 2021 12:20

Tgt Ion: 95 Resp: 20371
Ion Ratio Lower Upper
95 100
97 65.9 47.2 87.6
132 107.0 73.6 136.6
130 109.9 77.1 143.3


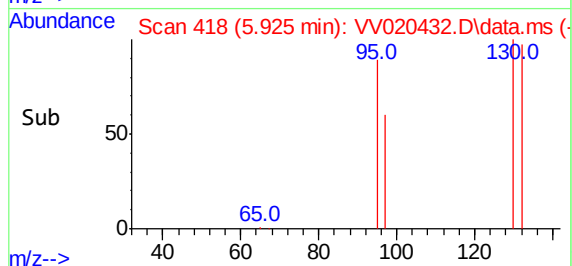
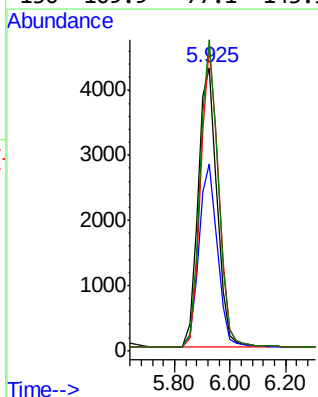
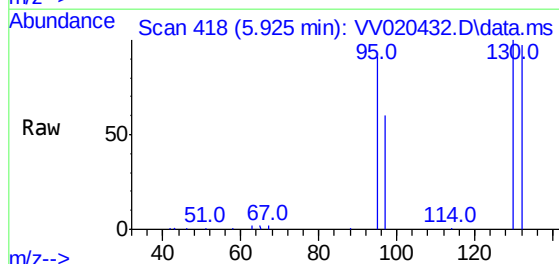


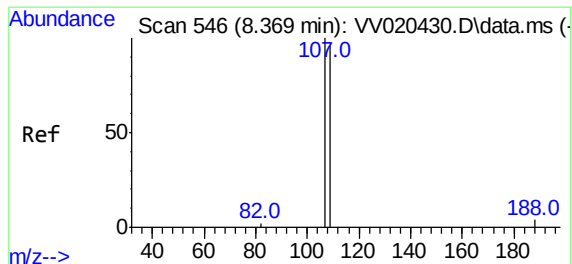

#9
1,2-Dibromoethane
Concen: 2.00 ug/L
RT: 8.353 min Scan# 545
Delta R.T. -0.015 min
Lab File: VV020432.D
Acq: 02 Mar 2021 12:20




Instrument :
MSVOA_V
ClientSampleId :
VSTD002306


Tgt Ion:107 Resp: 11762
Ion Ratio Lower Upper
107 100
109 91.8 67.3 125.1
188 5.0 7.8 11.8#

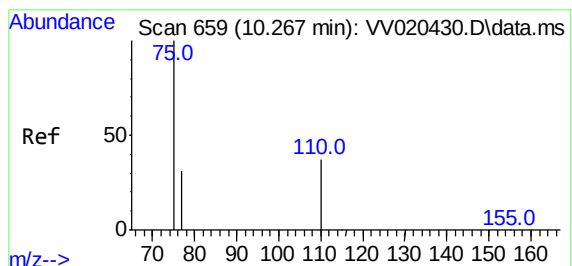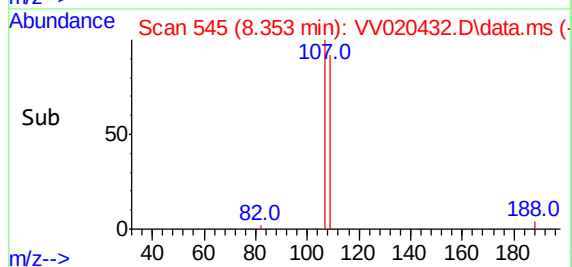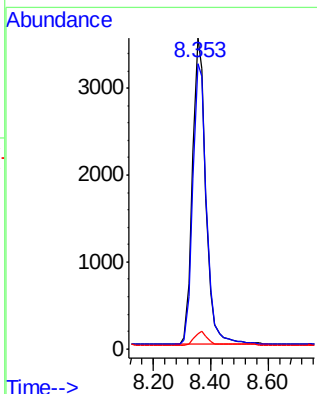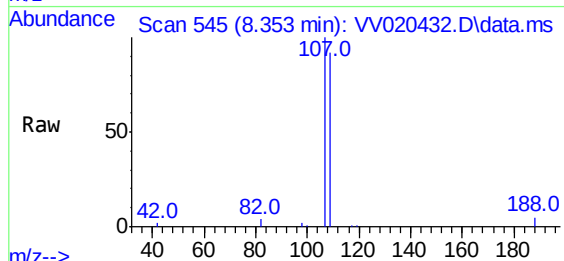

#12
1,2,3-Trichloropropane
Concen: 1.94 ug/L
RT: 10.267 min Scan# 659
Delta R.T. 0.000 min
Lab File: VV020432.D
Acq: 02 Mar 2021 12:20


Tgt Ion: 75 Resp: 10403
Ion Ratio Lower Upper
75 100
110 41.8 33.5 50.3
77 32.3 25.4 38.2

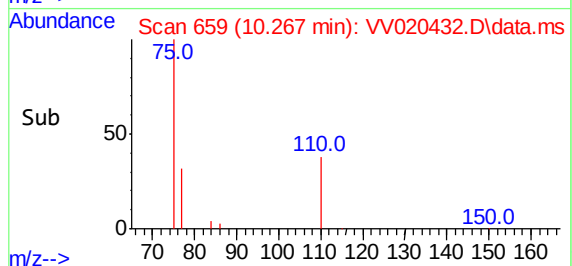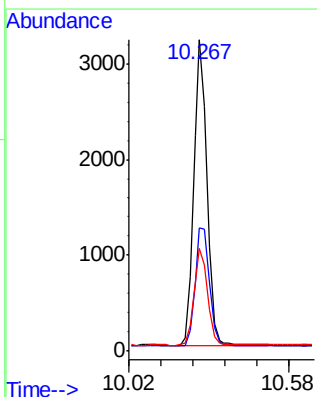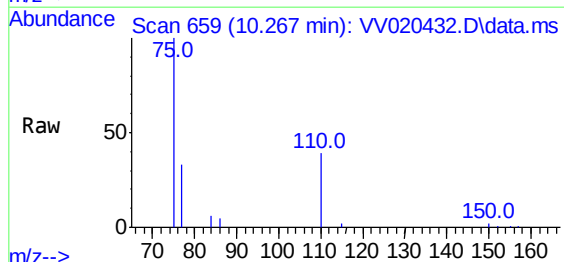

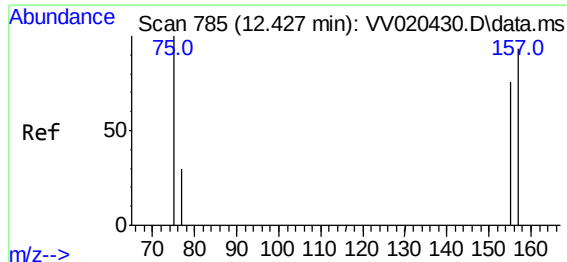

#13
 1,2-Dibromo-3-chloropropane
 Concen: 1.48 ug/L
 RT: 12.427 min Scan# 785
 Delta R.T. 0.000 min
 Lab File: VV020432.D
 Acq: 02 Mar 2021 12:20

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD002306

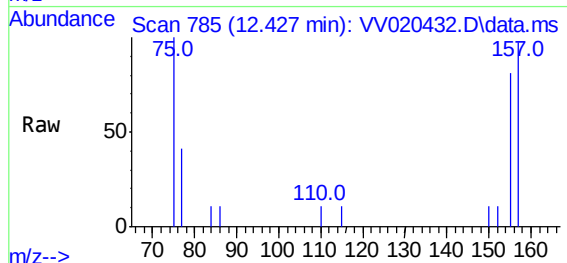

Tgt Ion: 75 Resp: 1337

Ion	Ratio	Lower	Upper
75	100		
157	97.4	74.3	111.5
155	81.1	65.4	98.2

