


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030221\
 Data File : VV020427.D
 Acq On : 02 Mar 2021 09:40
 Operator : SY/MD
 Sample : BFB34
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB307

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030221.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Mar 04 00:23:40 2021

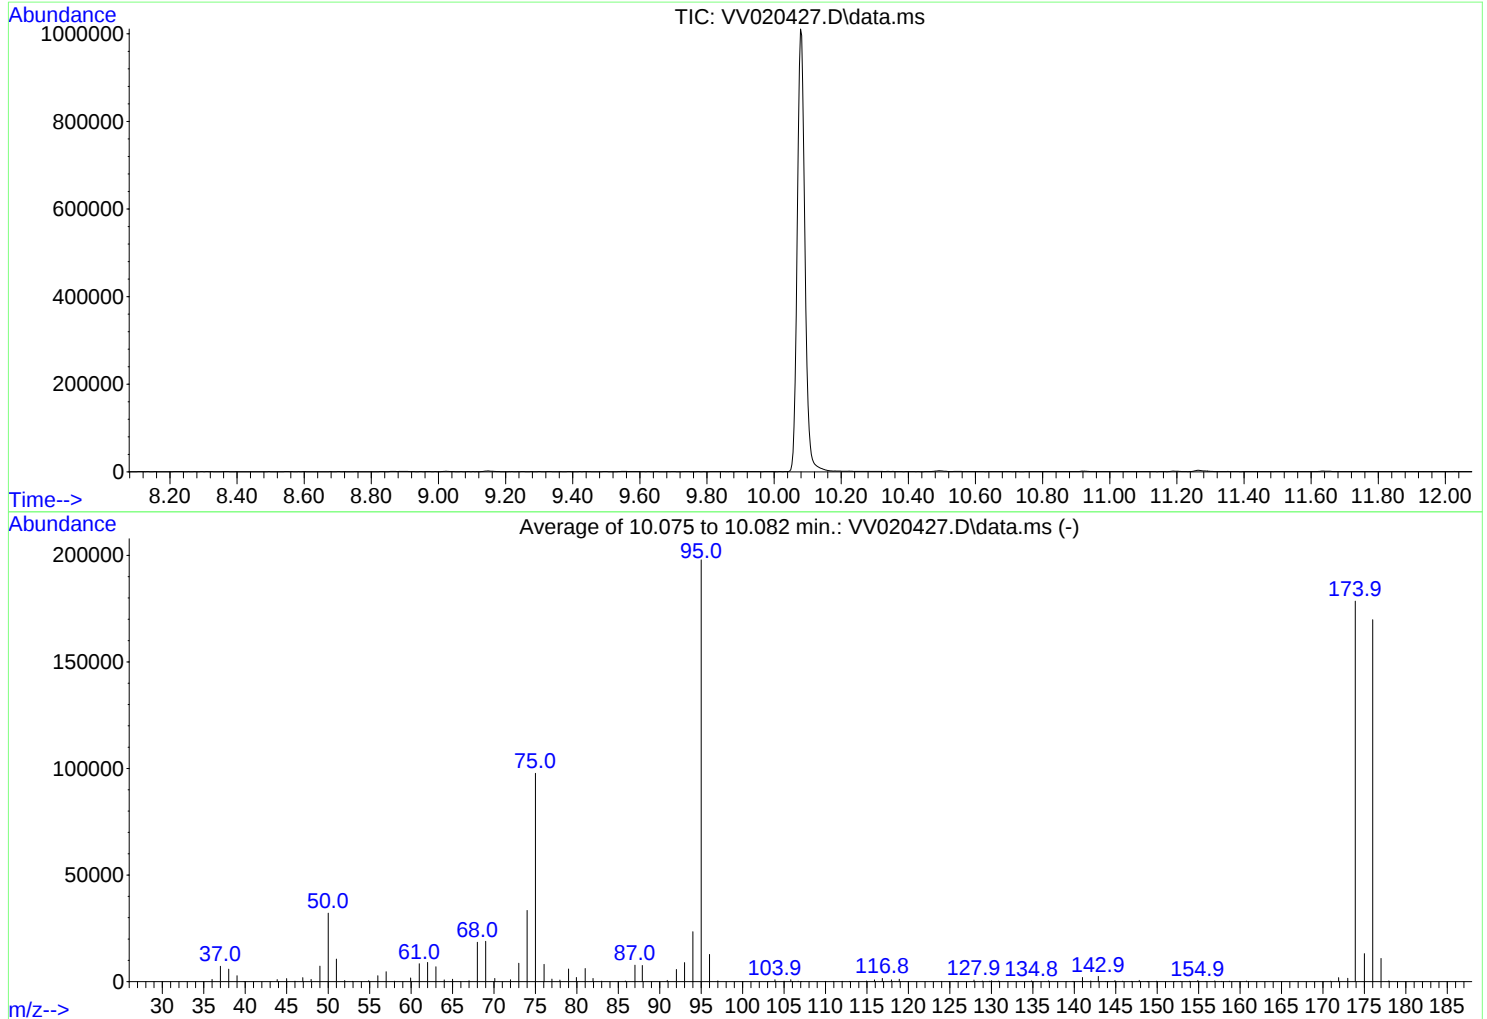

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	32112	PASS
75	95	30	80	49.4	97755	PASS
95	95	100	100	100.0	197888	PASS
96	95	5	9	6.5	12773	PASS
173	174	0.00	2	0.9	1616	PASS
174	95	50	120	90.2	178517	PASS
175	174	5	9	7.4	13180	PASS
176	174	95	101	95.1	169792	PASS
177	176	5	9	6.4	10861	PASS

m/z	Abundance
36.00	1096.0
37.00	7144.0
38.00	5812.0
39.00	2684.0
39.90	320.0
43.90	1305.0
45.00	1304.0
46.00	243.0
46.90	1651.0
48.00	891.0
49.00	6999.0
50.00	31192.0
51.00	10332.0
52.00	478.0
52.90	129.0
54.90	501.0
56.00	2472.0
57.00	4400.0
58.00	229.0
60.00	1787.0
61.00	8015.0
62.00	8556.0
63.00	6857.0
64.00	846.0
65.00	1145.0
67.00	445.0
68.00	17952.0
69.00	18184.0
70.10	1445.0
72.00	905.0
73.00	8288.0
74.00	31952.0
75.00	94168.0
76.10	7536.0
76.90	1102.0
78.00	775.0
79.00	5970.0
79.90	1958.0
81.00	5916.0
81.90	1398.0
83.00	204.0
85.90	305.0
87.00	7902.0
87.90	7099.0
90.90	592.0
92.00	5342.0
93.00	8658.0
94.00	22072.0
95.00	188288.0
96.00	12339.0
97.00	333.0
103.20	111.0
103.90	965.0
105.00	203.0
105.80	864.0
106.70	170.0
107.10	135.0
109.90	165.0
110.90	167.0
112.00	143.0
112.90	145.0
115.00	254.0
115.90	816.0
116.80	1443.0
118.00	798.0
118.90	1025.0
123.90	128.0
125.80	112.0
127.90	665.0
128.90	315.0
129.80	602.0
130.90	259.0
134.80	334.0
136.90	367.0
139.10	161.0
139.90	154.0
141.00	1820.0
142.00	213.0
142.90	2349.0
143.80	104.0
144.90	591.0
145.80	279.0
146.90	131.0
147.90	629.0
148.80	114.0
149.90	193.0
152.10	119.0
152.80	108.0
153.90	187.0
154.90	497.0
155.90	107.0
157.00	391.0

Instrument :
MSVOA_V
ClientSampleId :
BFB307

157.80	130.0
158.70	207.0
160.80	248.0
170.90	243.0
171.90	1722.0
173.00	1488.0
173.90	165952.0
175.00	12534.0
176.00	156800.0
177.00	10224.0
178.00	419.0

Instrument :
MSVOA_V
ClientSampleId :
BFB307

m/z	Abundance
36.00	1062.0
37.00	7510.0
38.00	5953.0
39.00	2864.0
39.90	327.0
43.10	110.0
43.90	1397.0
45.00	1403.0
46.00	213.0
47.00	1906.0
47.90	1069.0
49.00	7475.0
50.00	33280.0
51.00	11015.0
52.00	536.0
53.00	139.0
54.90	439.0
56.00	2853.0
57.00	4837.0
58.00	233.0
60.00	1794.0
61.00	8606.0
62.00	9355.0
63.00	7219.0
64.00	852.0
65.00	1139.0
65.90	104.0
67.00	441.0
68.00	19136.0
69.00	19496.0
70.10	1562.0
72.00	919.0
73.00	8935.0
74.00	34472.0
75.00	101152.0
76.00	8386.0
77.00	1218.0
78.00	741.0
79.00	6092.0
79.90	2067.0
81.00	6366.0
82.00	1541.0
83.00	204.0
85.90	332.0
87.00	7971.0
87.90	7868.0
90.90	633.0
92.00	5812.0
93.00	9292.0
94.00	24240.0
95.00	204736.0
96.00	13195.0
97.00	356.0
103.20	126.0
103.90	952.0
105.00	228.0
105.80	936.0
106.70	211.0
109.90	165.0
111.00	169.0
112.00	156.0
112.90	178.0
114.90	302.0
115.90	924.0
116.90	1552.0
118.00	813.0
118.90	1144.0
124.00	147.0
124.90	140.0
125.80	113.0
127.90	807.0
128.90	331.0
130.00	637.0
130.90	304.0
134.80	379.0
136.90	378.0
139.10	147.0
139.80	167.0
141.00	2024.0
142.00	300.0
142.90	2544.0
143.80	120.0
144.90	559.0
145.90	259.0
146.90	171.0
147.80	649.0
149.00	130.0
150.00	235.0
152.10	117.0
152.80	149.0
153.90	199.0
154.90	595.0

Instrument :
MSVOA_V
ClientSampleId :
BFB307

155.90	146.0
157.00	411.0
157.80	140.0
158.70	269.0
160.80	297.0
171.00	228.0
171.90	1908.0
173.00	1671.0
173.90	184640.0
175.00	13590.0
176.00	175744.0
177.00	11210.0
178.00	414.0

Instrument :
MSVOA_V
ClientSampleId :
BFB307

m/z	Abundance
36.00	984.0
37.00	7017.0
38.00	5831.0
39.00	2829.0
39.90	291.0
43.10	124.0
43.90	1359.0
45.00	1476.0
46.00	192.0
47.00	2046.0
47.90	1101.0
49.00	7341.0
50.00	31864.0
51.00	10454.0
52.00	509.0
53.00	138.0
54.90	355.0
56.00	2923.0
57.00	4665.0
58.00	181.0
59.90	1659.0
61.00	8603.0
62.00	9095.0
63.00	6980.0
64.00	776.0
65.00	1161.0
66.00	131.0
67.00	442.0
68.00	18392.0
69.00	19072.0
70.10	1451.0
72.00	882.0
73.00	8619.0
74.00	33720.0
75.00	97944.0
76.00	8433.0
77.10	1213.0
77.90	785.0
79.00	5695.0
80.00	1934.0
81.00	6158.0
81.90	1543.0
83.00	204.0
85.80	266.0
87.00	7400.0
87.90	7775.0
90.90	673.0
92.00	5921.0
93.00	8792.0
94.00	23912.0
95.00	200640.0
96.00	12786.0
97.00	370.0
103.10	111.0
103.90	866.0
105.00	234.0
105.80	863.0
106.70	216.0
110.00	154.0
110.90	149.0
112.00	147.0
112.90	173.0
114.90	298.0
115.90	849.0
116.90	1527.0
117.80	824.0
118.90	1180.0
124.00	121.0
124.90	181.0
125.80	112.0
127.90	839.0
128.90	330.0
130.00	700.0
130.90	318.0
134.90	417.0
136.90	368.0
139.80	162.0
141.00	2063.0
142.00	319.0
142.90	2506.0
144.00	117.0
144.90	456.0
145.90	250.0
146.90	157.0
147.80	553.0
148.90	163.0
150.00	260.0
152.90	187.0
153.90	191.0
154.90	617.0
155.90	154.0
156.90	388.0

Instrument :
MSVOA_V
ClientSampleId :
BFB307

157.80	104.0
158.70	260.0
160.80	354.0
170.90	175.0
171.90	1951.0
173.00	1688.0
173.90	184960.0
175.00	13417.0
176.00	176832.0
177.00	11149.0
177.90	326.0

Instrument :
MSVOA_V
ClientSampleId :
BFB307

m/z	Abundance
39.80	204.0
43.80	395.0

Instrument :
MSVOA_V
ClientSampleId :
BFB307