




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
 Data File : VV030120.D
 Acq On : 02 Mar 2023 14:41
 Operator : SY/MD
 Sample : 01769-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBYL2

Manual IntegrationsAPPROVED

Quant Time: Mar 03 03:32:25 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 03 03:28:37 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/03/2023
 Supervised By :Mahesh Dadoda 03/03/2023

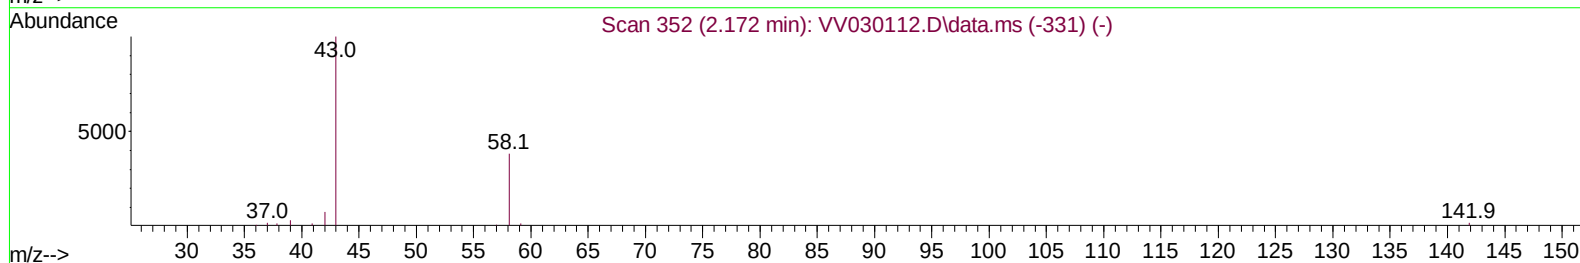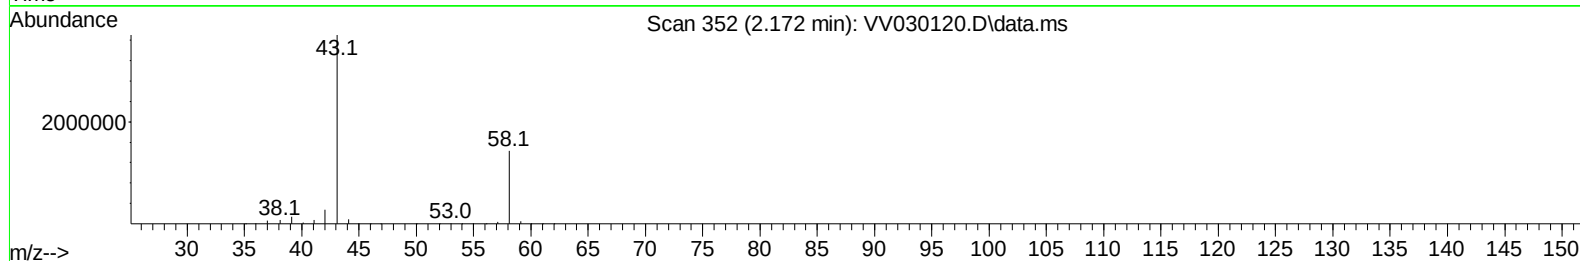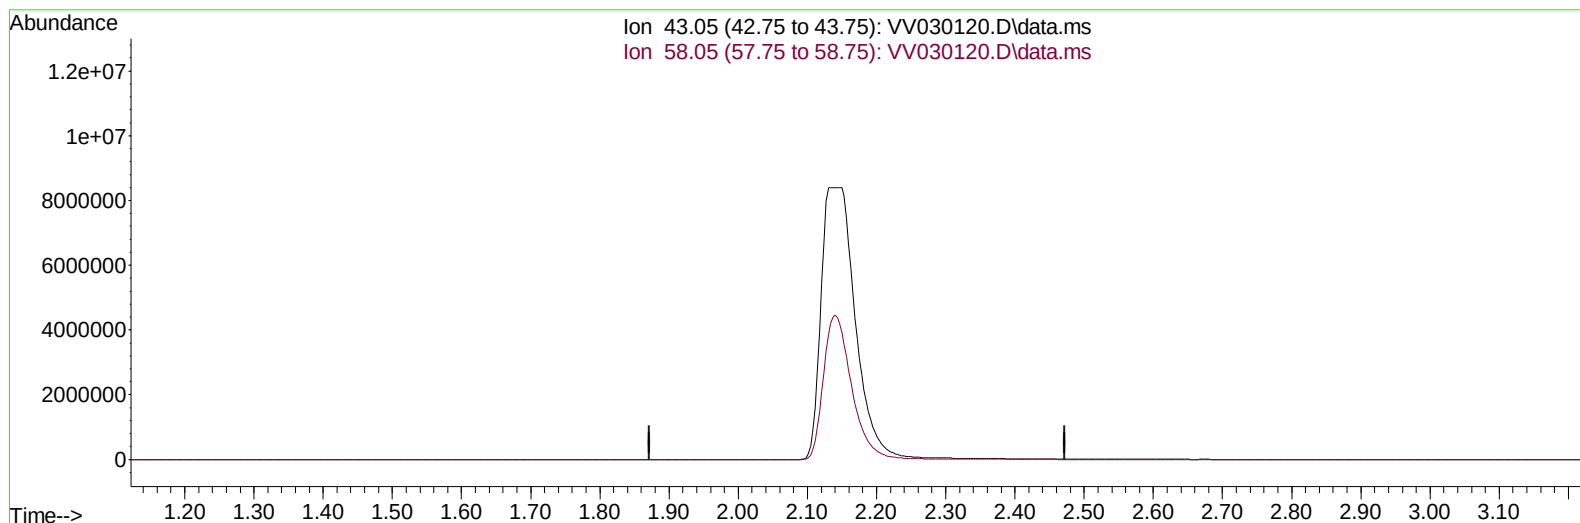

TIC: VV030120.D\data.ms

(13) Acetone (T)

2.172min (-2.172) 0.00 ug/L

response 0

Ion	Exp%	Act%
43.05	100.00	0.00
58.05	14.70	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
 Data File : VV030120.D
 Acq On : 02 Mar 2023 14:41
 Operator : SY/MD
 Sample : 01769-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBYL2

Manual IntegrationsAPPROVED

Quant Time: Mar 03 03:32:25 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 03 03:28:37 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/03/2023
 Supervised By :Mahesh Dadoda 03/03/2023

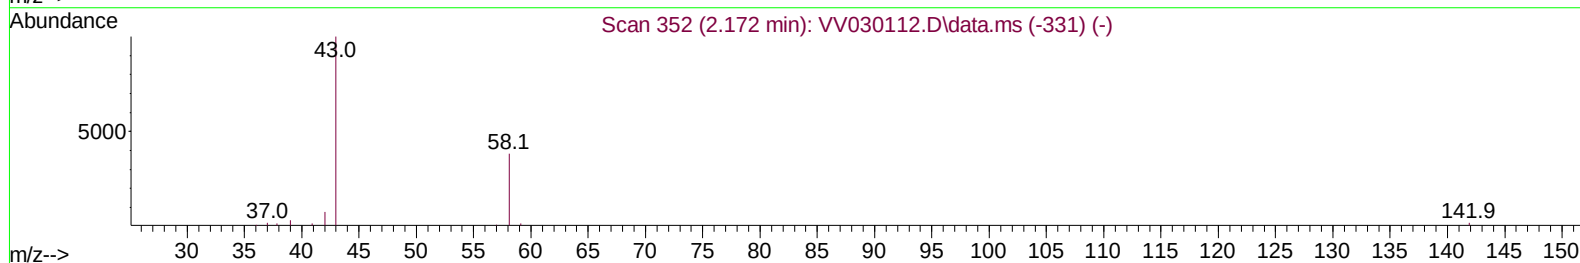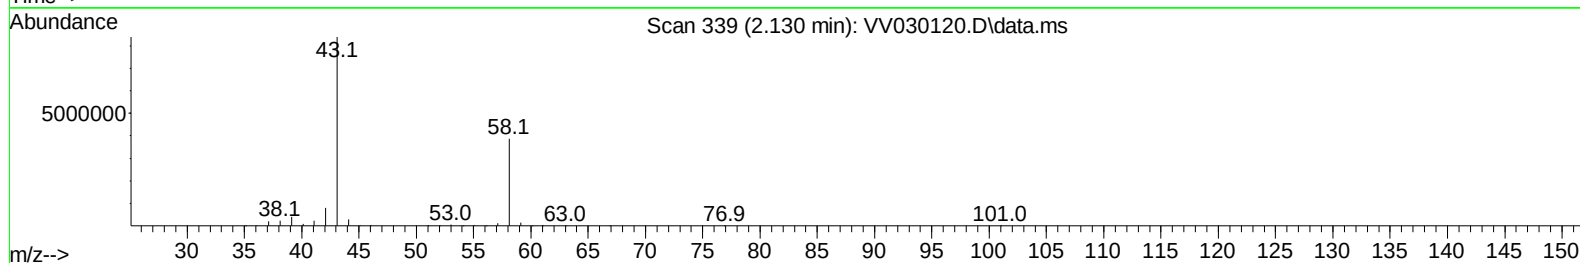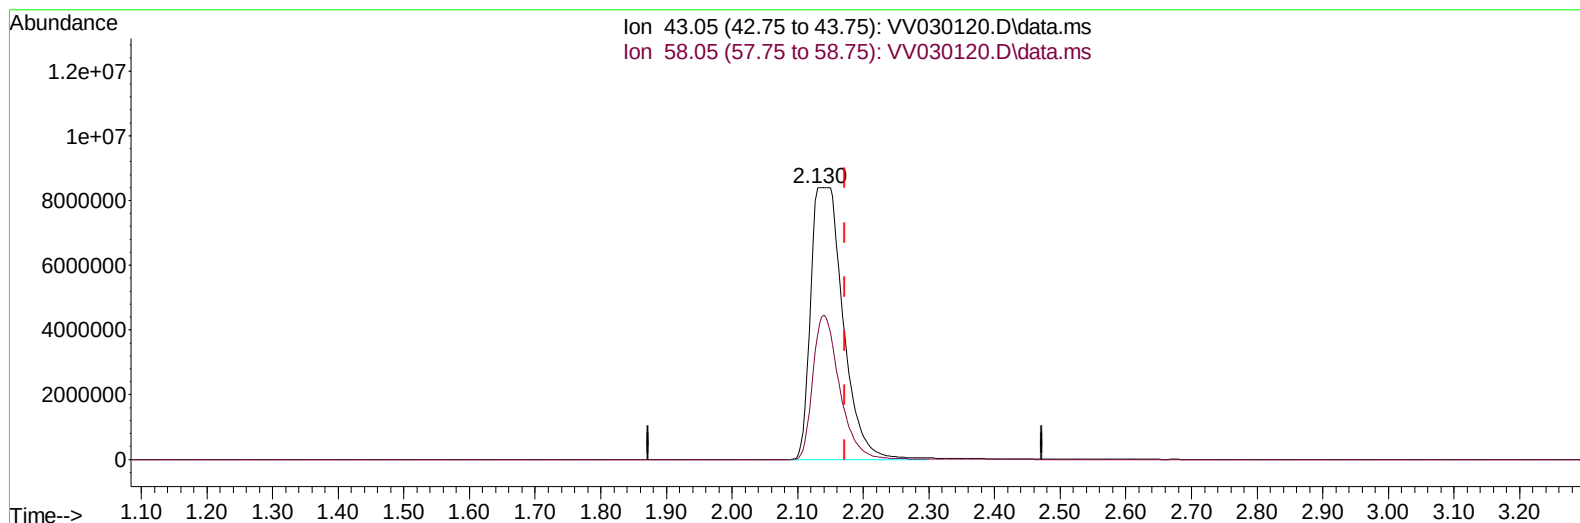

TIC: VV030120.D\data.ms

(13) Acetone (T)

2.130min (-0.042) 21068.47 ug/L m

response 28741414

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	14.70	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
 Data File : VV030120.D
 Acq On : 02 Mar 2023 14:41
 Operator : SY/MD
 Sample : 01769-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBYL2

Manual IntegrationsAPPROVED

Quant Time: Mar 03 03:32:25 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 03 03:28:37 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/03/2023
 Supervised By :Mahesh Dadoda 03/03/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.545	114		154717	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117		154536	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152		76333	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.282	65		43954	4.391	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.800%	
7) Chloroethane-d5	1.539	69		46792	4.979	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.600%	
11) 1,1-Dichloroethene-d2	2.066	63		73515	3.572	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.400%	
20) 2-Butanone-d5	3.815	46		94754	51.337	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.680%	
24) Chloroform-d	4.262	84		100558	4.917	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.400%	
26) 1,2-Dichloroethane-d4	4.953	65		44848	5.372	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.400%	
32) Benzene-d6	4.973	84		188310	4.529	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.600%	
36) 1,2-Dichloropropane-d6	5.998	67		61188	4.891	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.800%	
41) Toluene-d8	7.252	98		158982	4.033	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.600%	
43) trans-1,3-Dichloroprop...	7.561	79		19024	4.445	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.800%	
46) 2-Hexanone-d5	8.034	63		87029	49.151	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.300%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84		45572	5.121	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.400%	
66) 1,2-Dichlorobenzene-d4	11.570	152		65806	5.095	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.000%	
Target Compounds							
13) Acetone	2.130	43	28741414m	21068.469	ug/L		Qvalue
14) Carbon disulfide	2.246	76	6479	0.233	ug/L		99
42) Toluene	7.333	91	4727	0.103	ug/L		84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030120.D
Acq On : 02 Mar 2023 14:41
Operator : SY/MD
Sample : 01769-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBYL2

Manual IntegrationsAPPROVED

Quant Time: Mar 03 03:32:25 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 03 03:28:37 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 03/03/2023
Supervised By :Mahesh Dadoda 03/03/2023

