




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
 Data File : VV030124.D
 Acq On : 02 Mar 2023 17:47
 Operator : SY/MD
 Sample : 01769-04 500X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBYL4

Manual IntegrationsAPPROVED

Quant Time: Mar 03 03:33:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 03 03:28:37 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/03/2023
 Supervised By :Mahesh Dadoda 03/03/2023

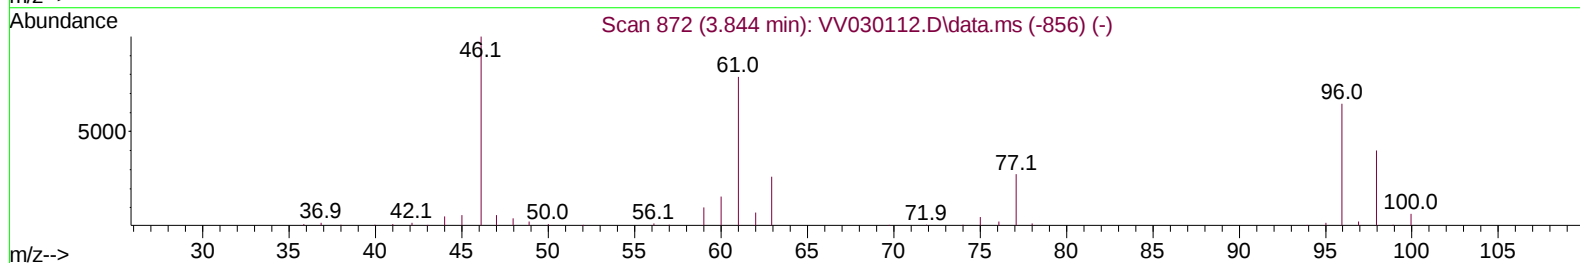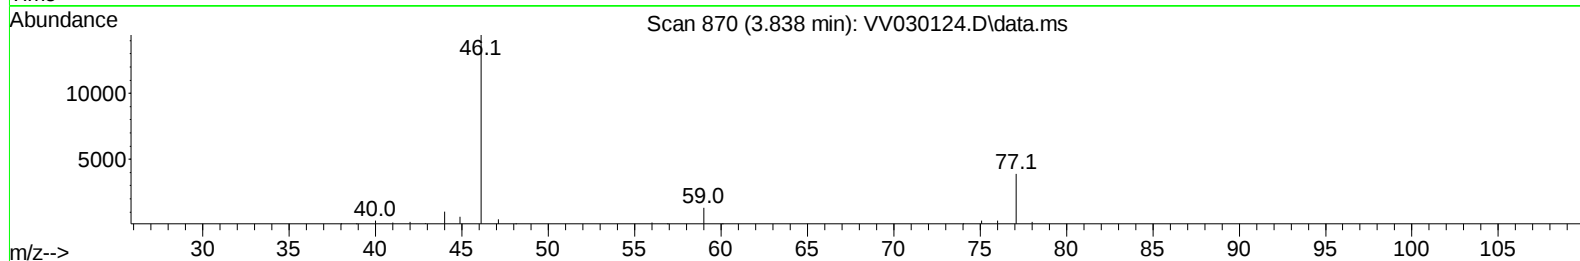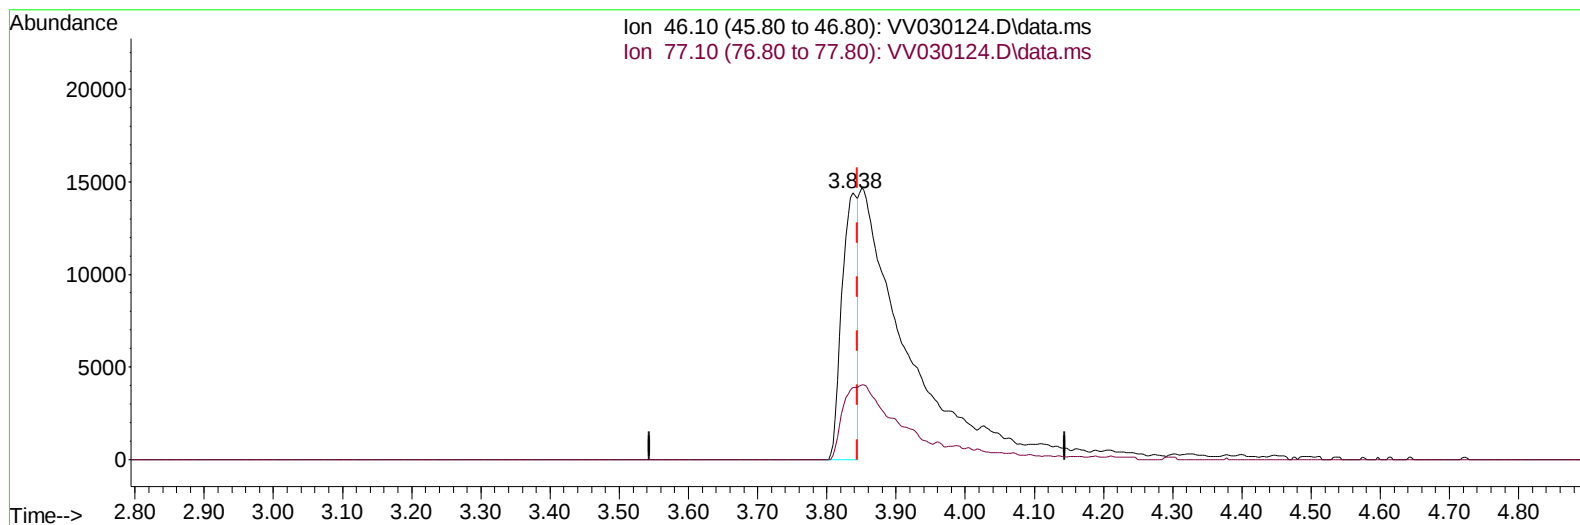

TIC: VV030124.D\data.ms

(20) 2-Butanone-d5 (S)

3.838min (-0.007) 13.41 ug/L

response 22325

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	12.60	93.26#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
 Data File : VV030124.D
 Acq On : 02 Mar 2023 17:47
 Operator : SY/MD
 Sample : 01769-04 500X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBYL4

Manual IntegrationsAPPROVED

Quant Time: Mar 03 03:33:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 03 03:28:37 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/03/2023
 Supervised By :Mahesh Dadoda 03/03/2023

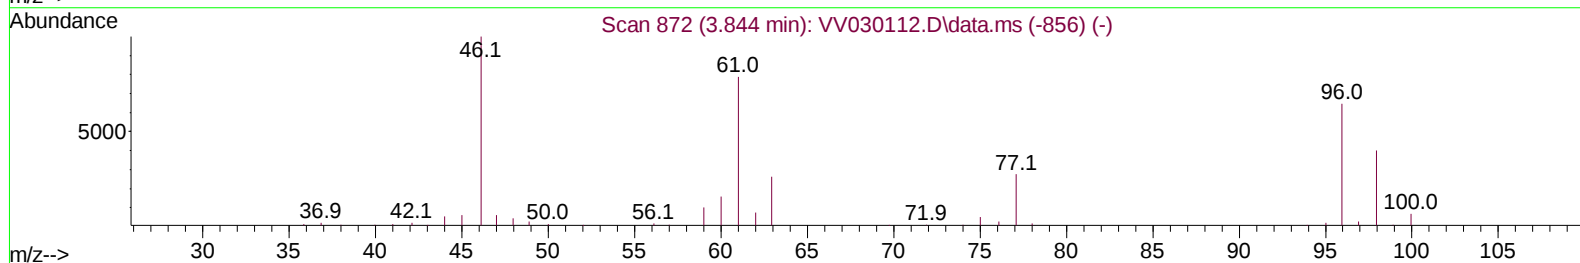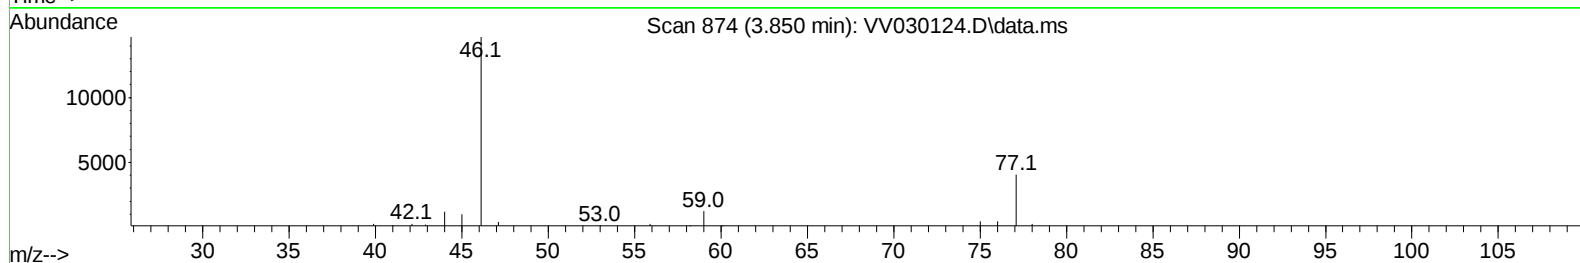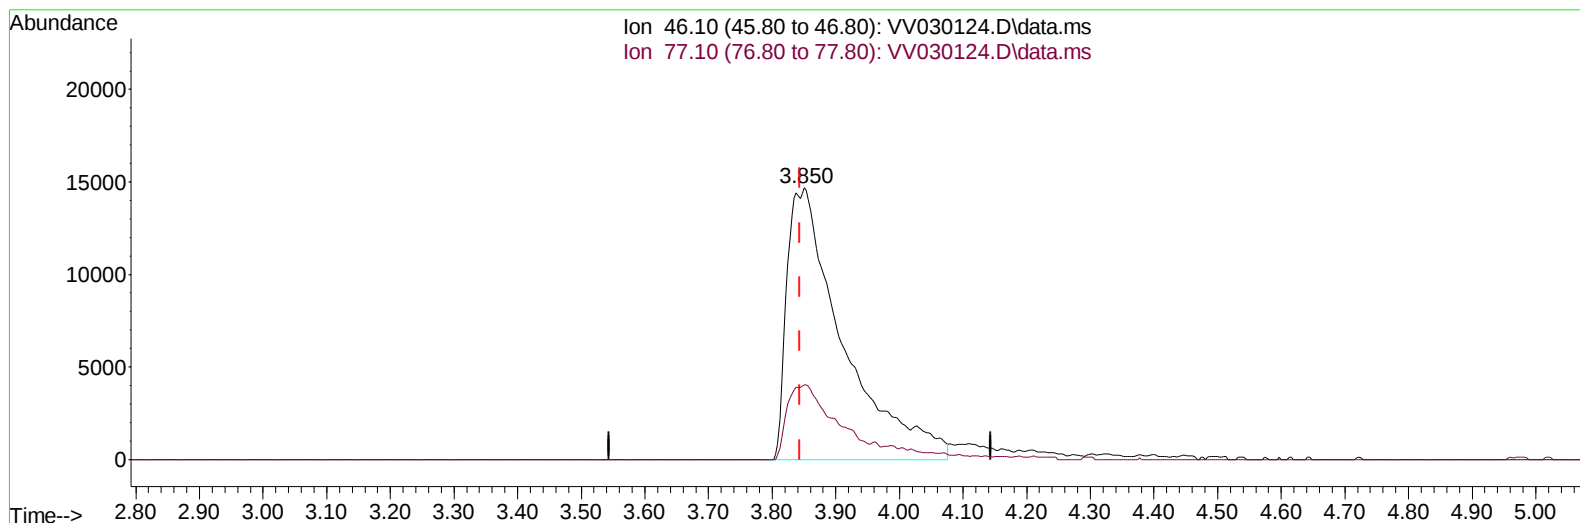

TIC: VV030124.D\data.ms

(20) 2-Butanone-d5 (S)

3.850min (+ 0.006) 53.76 ug/L m

response 89485

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	12.60	23.27#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
 Data File : VV030124.D
 Acq On : 02 Mar 2023 17:47
 Operator : SY/MD
 Sample : 01769-04 500X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBYL4

Manual IntegrationsAPPROVED

Quant Time: Mar 03 03:33:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 03 03:28:37 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/03/2023
 Supervised By :Mahesh Dadoda 03/03/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	139541	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	138971	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	67747	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	39503	4.375	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	87.600%		
7) Chloroethane-d5	1.535	69	41419	4.887	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	97.800%		
11) 1,1-Dichloroethene-d2	2.063	63	64607	3.481	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	69.600%		
20) 2-Butanone-d5	3.850	46	89485m	53.755	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	107.520%		
24) Chloroform-d	4.262	84	92556	5.018	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	100.400%		
26) 1,2-Dichloroethane-d4	4.957	65	40751	5.412	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	108.200%		
32) Benzene-d6	4.973	84	168996	4.519	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	90.400%		
36) 1,2-Dichloropropane-d6	5.998	67	55342	4.919	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	98.400%		
41) Toluene-d8	7.252	98	139711	3.942	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	78.800%		
43) trans-1,3-Dichloroprop...	7.564	79	16852	4.378	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	87.600%		
46) 2-Hexanone-d5	8.040	63	79632	50.010	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	100.020%		
56) 1,1,2,2-Tetrachloroeth...	10.162	84	42532	5.314	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	106.200%		
66) 1,2-Dichlorobenzene-d4	11.570	152	55779	4.866	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	97.400%		
Target Compounds						
						Qvalue
16) Methylene chloride	2.455	84	4642	0.406	ug/L	92
72) 1,2,3-Trichlorobenzene	13.689	180	993	0.089	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030124.D
Acq On : 02 Mar 2023 17:47
Operator : SY/MD
Sample : 01769-04 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
DBYL4

Manual IntegrationsAPPROVED

Quant Time: Mar 03 03:33:24 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 03 03:28:37 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 03/03/2023
Supervised By :Mahesh Dadoda 03/03/2023

