

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
 Data File : VV030121.D
 Acq On : 02 Mar 2023 15:09
 Operator : SY/MD
 Sample : VIBLK274
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK274

Quant Time: Mar 03 03:32:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 03 03:28:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	143821	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	145002	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	72273	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	42240	4.539	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.800%
7) Chloroethane-d5	1.539	69	44850	5.134	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.600%
11) 1,1-Dichloroethene-d2	2.066	63	68872	3.600	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.000%
20) 2-Butanone-d5	3.818	46	88354	51.496	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.000%
24) Chloroform-d	4.259	84	98085	5.160	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.200%
26) 1,2-Dichloroethane-d4	4.953	65	43864	5.652	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	113.000%
32) Benzene-d6	4.969	84	179620	4.604	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.000%
36) 1,2-Dichloropropane-d6	5.998	67	59146	5.039	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.800%
41) Toluene-d8	7.252	98	150941	4.081	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.600%
43) trans-1,3-Dichloroprop...	7.561	79	17897	4.457	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.200%
46) 2-Hexanone-d5	8.034	63	80220	48.284	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.560%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	43795	5.245	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.800%
66) 1,2-Dichlorobenzene-d4	11.570	152	60788	4.971	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.400%
Target Compounds						
					Qvalue	
13) Acetone	2.150	43	38165	30.096	ug/L	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030121.D
Acq On : 02 Mar 2023 15:09
Operator : SY/MD
Sample : VIBLK274
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK274

Quant Time: Mar 03 03:32:39 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 03 03:28:37 2023
Response via : Initial Calibration

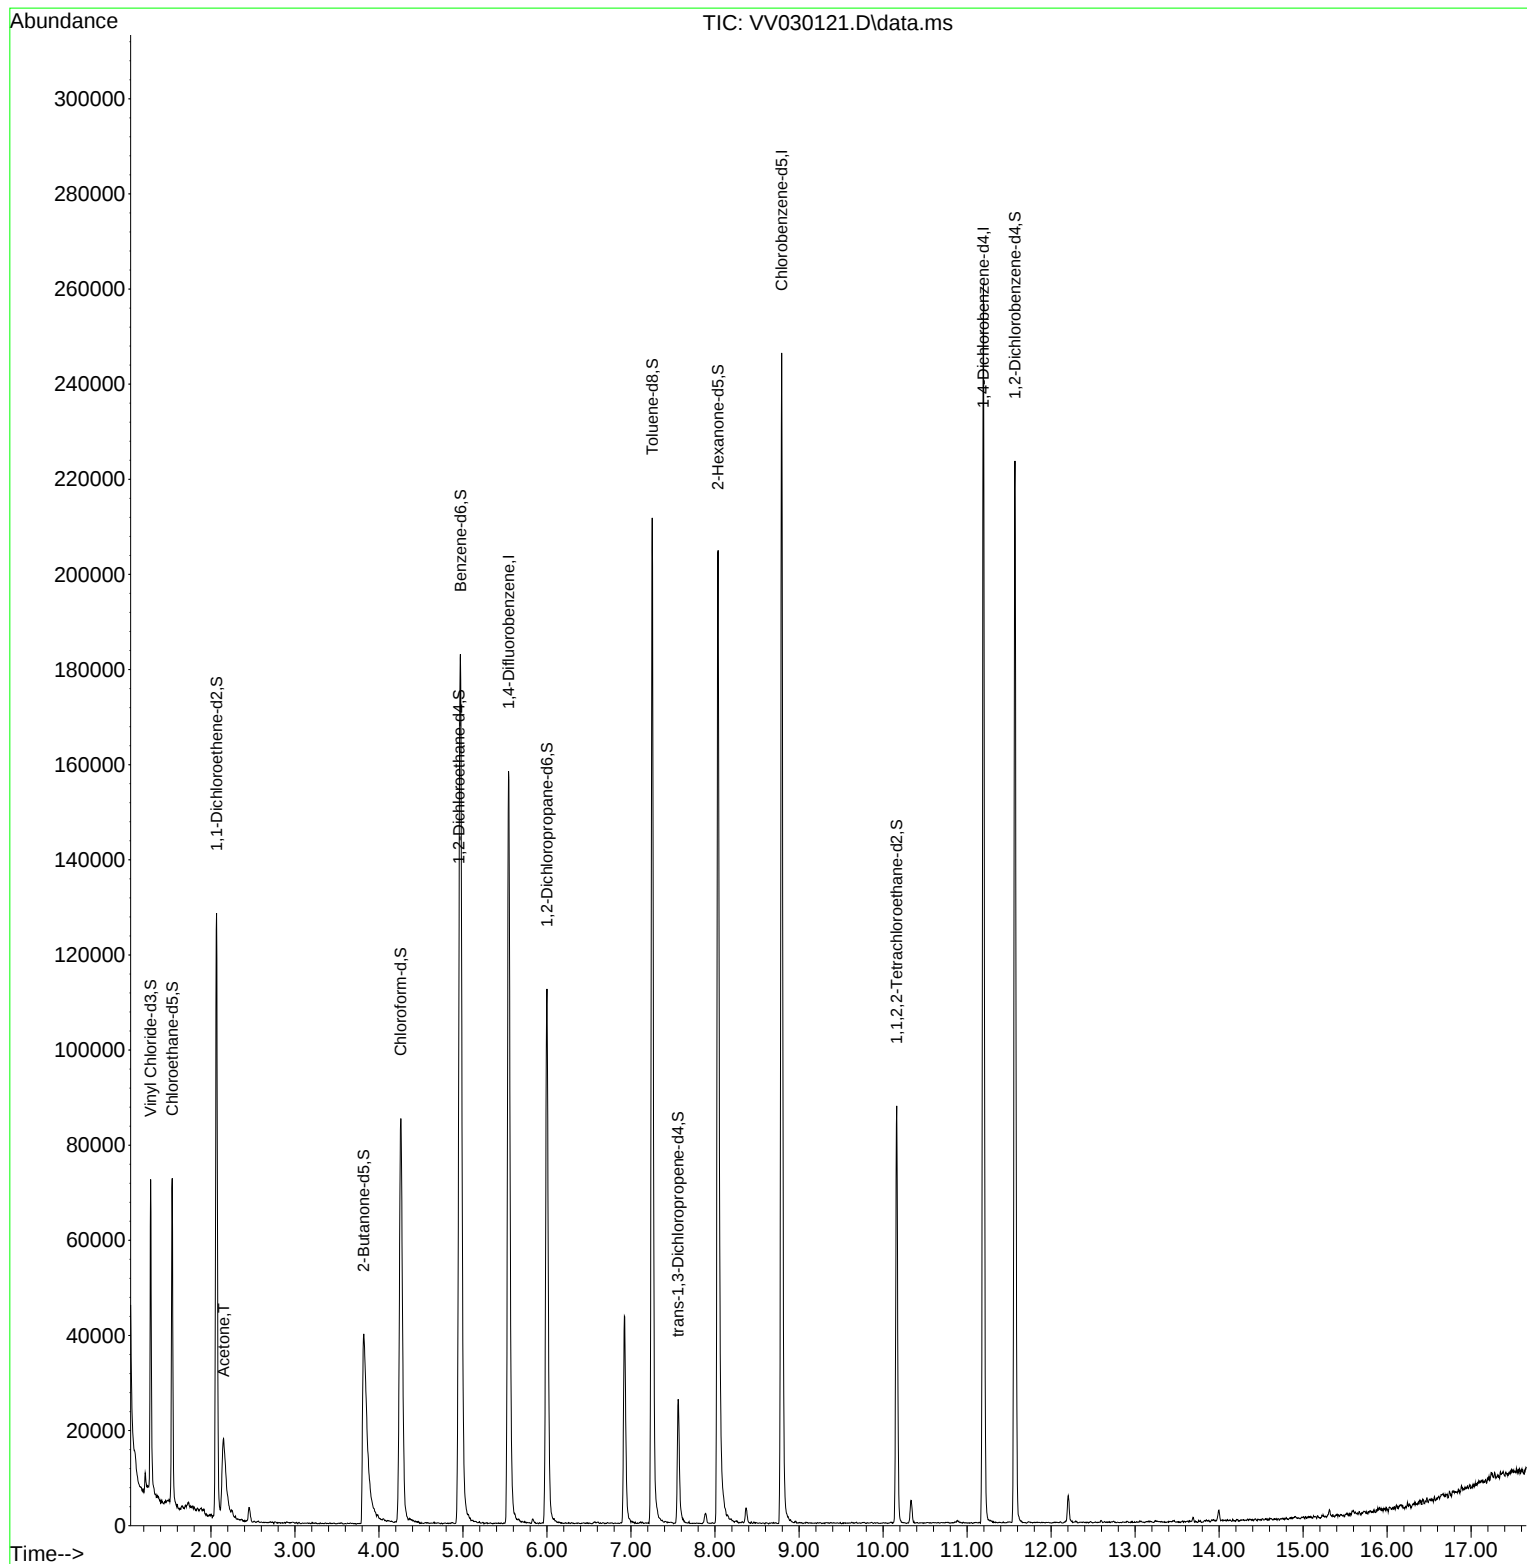

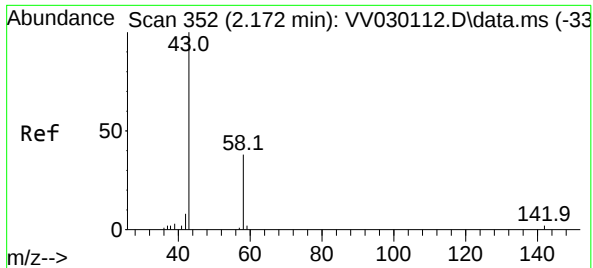

#13
 Acetone
 Concen: 30.096 ug/L
 RT: 2.150 min Scan# 34
 Delta R.T. -0.023 min
 Lab File: VV030121.D
 Acq: 02 Mar 2023 15:09

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK274

Tgt Ion: 43 Resp: 38165
 Ion Ratio Lower Upper
 43 100
 58 29.2 0.0 29.4

