

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
 Data File : VV030125.D
 Acq On : 02 Mar 2023 18:11
 Operator : SY/MD
 Sample : 01769-05 500X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBYL5

Quant Time: Mar 03 03:33:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 03 03:28:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	139794	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	137330	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	66249	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	38650	4.273	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.400%
7) Chloroethane-d5	1.535	69	41218	4.854	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.000%
11) 1,1-Dichloroethene-d2	2.063	63	65043	3.498	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.000%
20) 2-Butanone-d5	3.841	46	81876	49.095	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.200%
24) Chloroform-d	4.262	84	94341	5.106	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.200%
26) 1,2-Dichloroethane-d4	4.953	65	41209	5.463	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.200%
32) Benzene-d6	4.973	84	170973	4.627	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.600%
36) 1,2-Dichloropropane-d6	5.998	67	55163	4.962	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.200%
41) Toluene-d8	7.252	98	138541	3.955	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.200%
43) trans-1,3-Dichloroprop...	7.564	79	16791	4.415	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.200%
46) 2-Hexanone-d5	8.037	63	76552	48.650	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.300%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	42273	5.345	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.000%
66) 1,2-Dichlorobenzene-d4	11.570	152	55555	4.956	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.200%
Target Compounds						Qvalue
16) Methylene chloride	2.455	84	7030	0.613	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030125.D
Acq On : 02 Mar 2023 18:11
Operator : SY/MD
Sample : 01769-05 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBYL5

Quant Time: Mar 03 03:33:38 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 03 03:28:37 2023
Response via : Initial Calibration

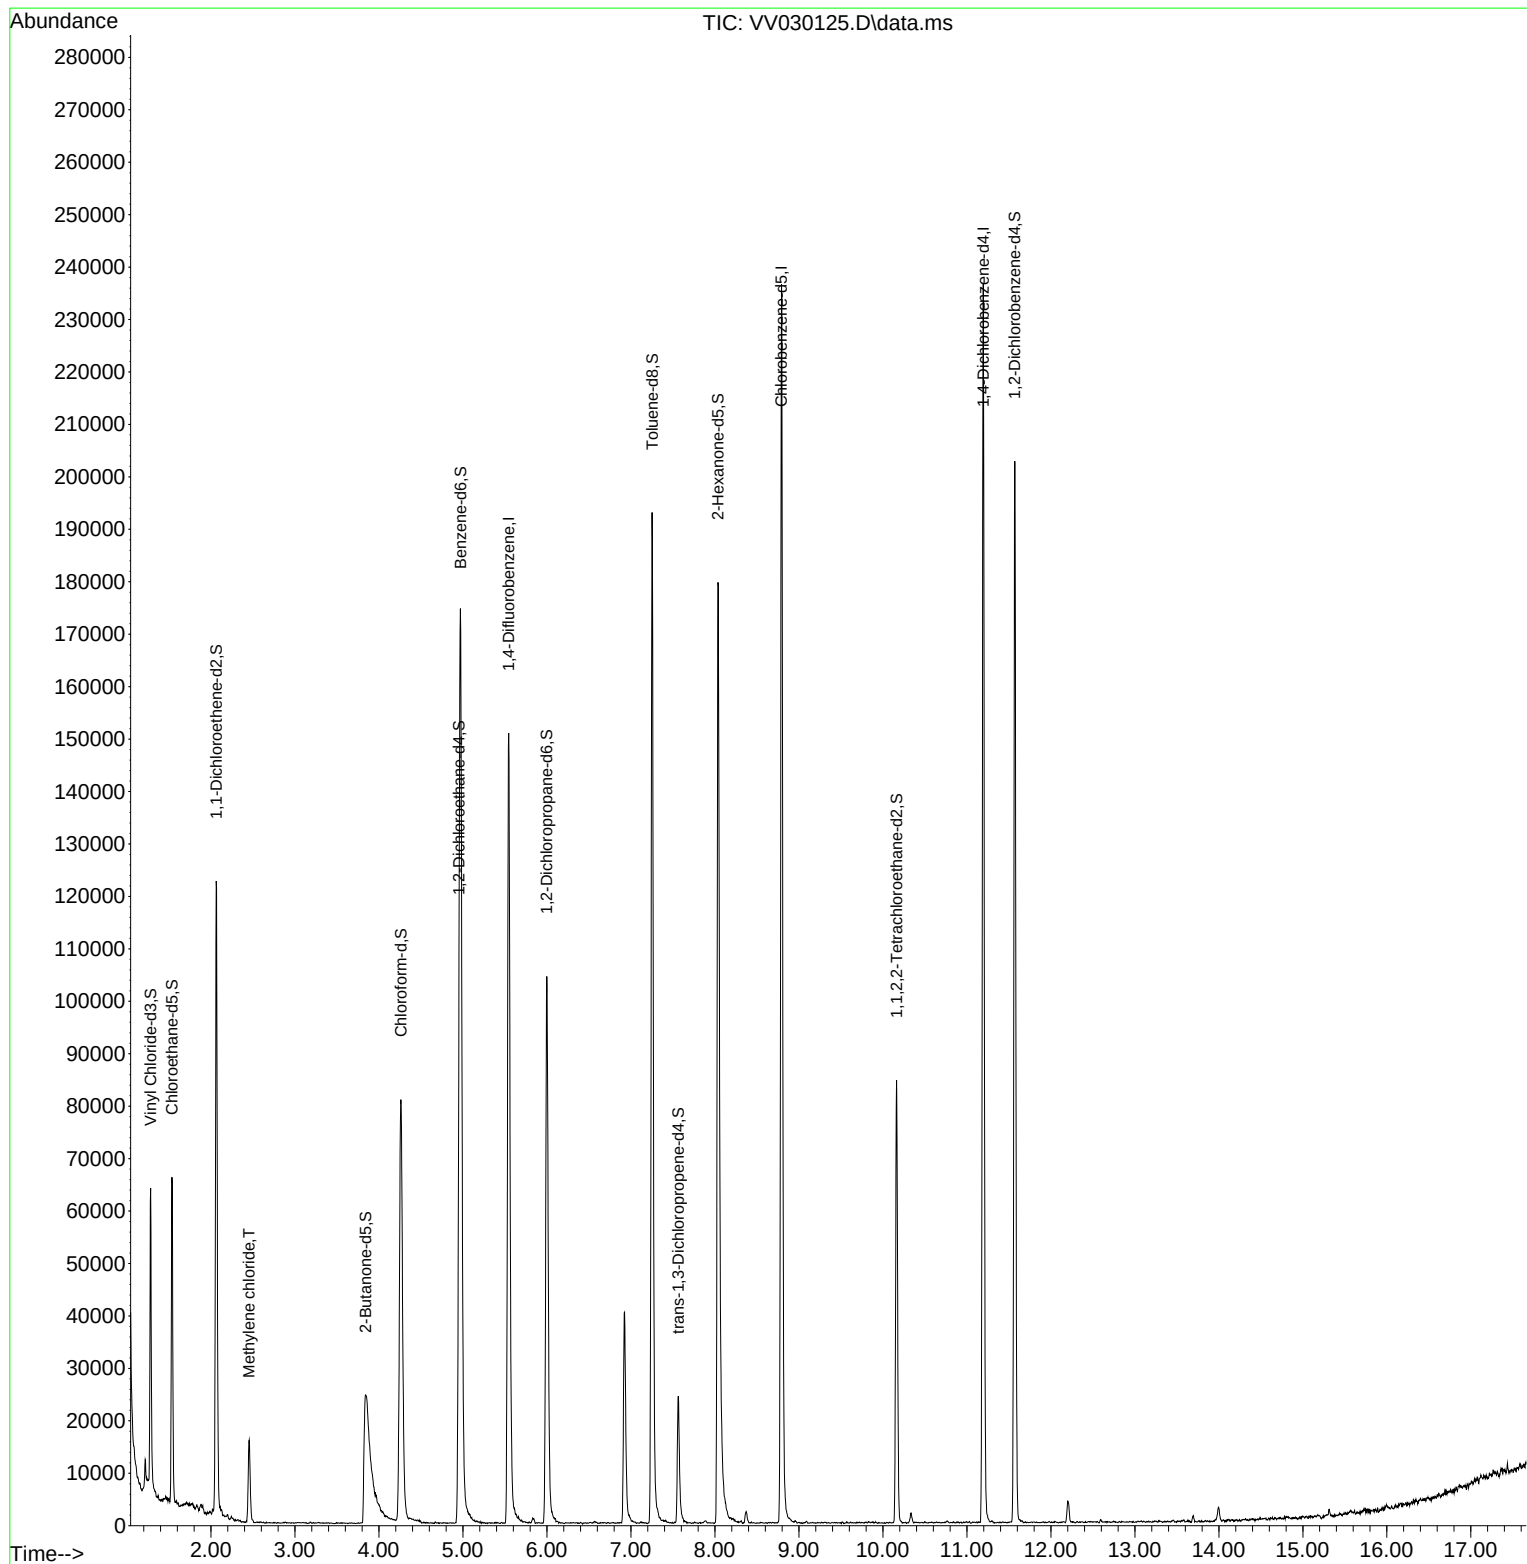

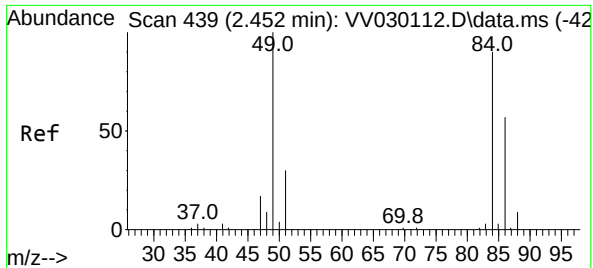

#16
Methylene chloride
Concen: 0.613 ug/L
RT: 2.455 min Scan# 44
Delta R.T. 0.003 min
Lab File: VV030125.D
Acq: 02 Mar 2023 18:11

Instrument :
MSVOA_V
ClientSampleId :
DBYL5

Tgt Ion: 84 Resp: 7030
Ion Ratio Lower Upper
84 100
86 64.2 44.7 83.1
49 111.8 78.8 146.3

