

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
 Data File : VV030113.D
 Acq On : 02 Mar 2023 10:31
 Operator : SY/MD
 Sample : VV0302WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK306

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030113.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	90	rVB	67165	74207	15.45%	1.881%
2	1.536	147	154	167	rVB	72837	84591	17.61%	2.144%
3	2.063	309	318	339	rBV	137702	198701	41.37%	5.037%
4	2.455	431	440	450	rBV3	3808	5853	1.22%	0.148%
5	3.854	859	875	897	rBV2	21643	102636	21.37%	2.602%
6	4.259	985	1001	1032	rBV2	85775	221955	46.21%	5.627%
7	4.970	1203	1222	1250	rBV3	190045	480337	100.00%	12.177%
8	5.545	1385	1401	1425	rBV	156579	325792	67.83%	8.259%
9	5.998	1528	1542	1565	rBV	112926	239252	49.81%	6.065%
10	6.924	1819	1830	1854	rBV2	44355	85820	17.87%	2.176%
11	7.252	1920	1932	1962	rBV	213736	383301	79.80%	9.717%
12	7.564	2016	2029	2052	rBV	27034	49932	10.40%	1.266%
13	8.040	2165	2177	2208	rBV	189304	397211	82.69%	10.070%
14	8.793	2400	2411	2440	rBV	238801	403303	83.96%	10.224%
15	10.162	2825	2837	2858	rBV	91048	144038	29.99%	3.652%
16	11.194	3145	3158	3181	rBV	250840	389173	81.02%	9.866%
17	11.571	3261	3275	3293	rBV	224143	351951	73.27%	8.922%
18	12.204	3462	3472	3482	rBV	4206	6504	1.35%	0.165%




Sum of corrected areas: 3944557

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030113.D
Acq On : 02 Mar 2023 10:31
Operator : SY/MD
Sample : VV0302WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK306

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

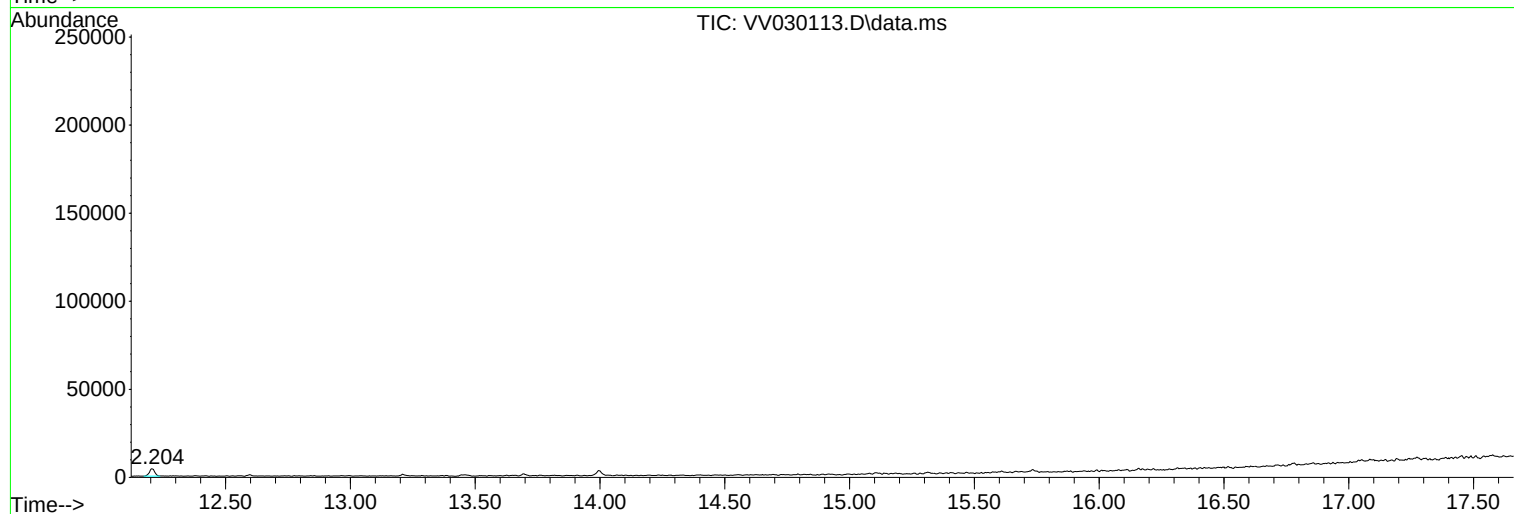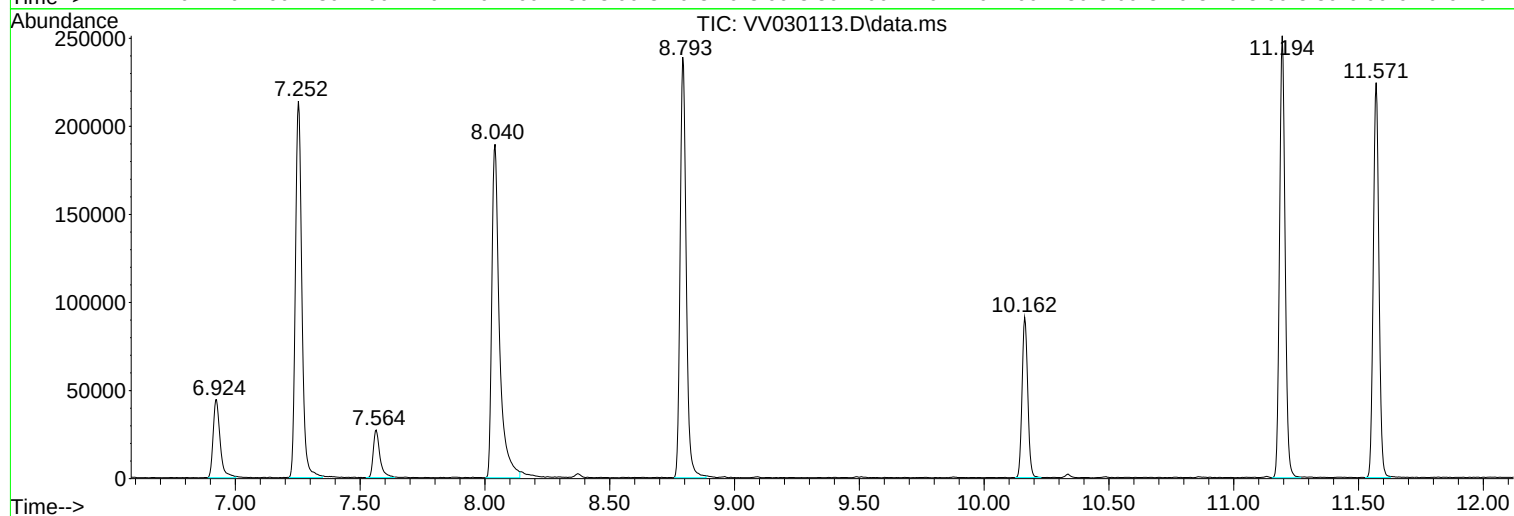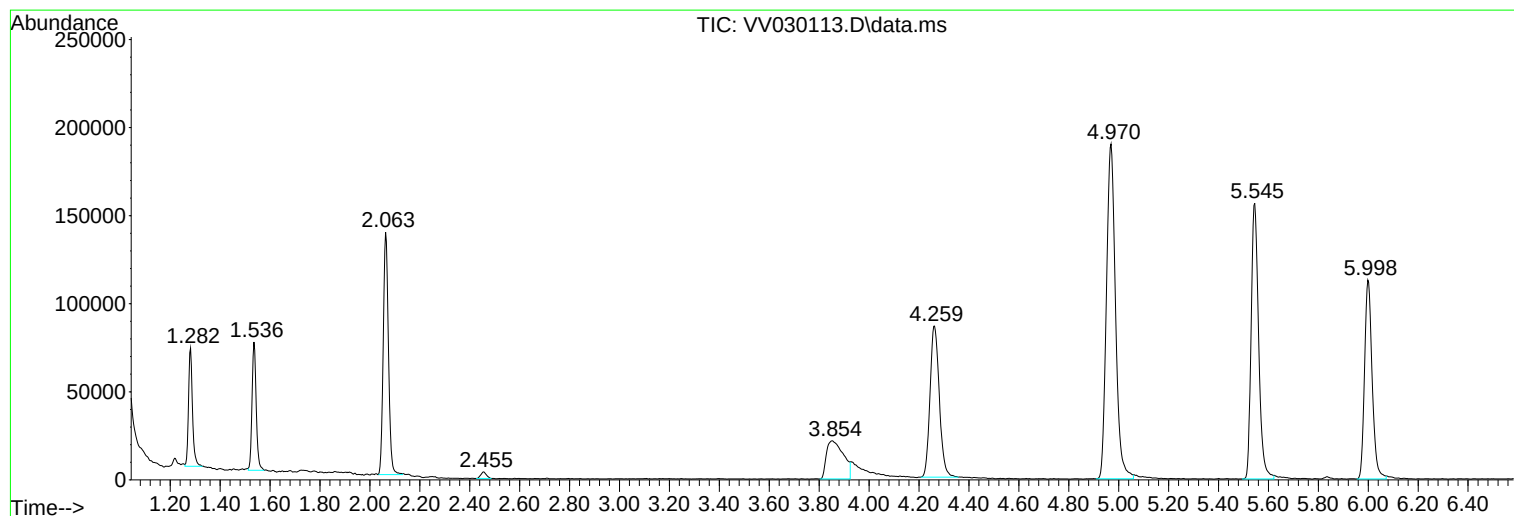

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030113.D
Acq On : 02 Mar 2023 10:31
Operator : SY/MD
Sample : VV0302WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK306

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030113.D
Acq On : 02 Mar 2023 10:31
Operator : SY/MD
Sample : VV0302WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK306

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc