

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
 Data File : VV030114.D
 Acq On : 02 Mar 2023 11:54
 Operator : SY/MD
 Sample : 01729-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BY9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030114.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	52	56	63	rVB	7959	7940	1.64%	0.182%
2	1.282	68	75	93	rVB	71702	86209	17.81%	1.973%
3	1.388	103	108	117	rVB	11706	14071	2.91%	0.322%
4	1.539	147	155	170	rVB	71704	86022	17.77%	1.969%
5	2.066	308	319	336	rBV	131862	195398	40.37%	4.473%
6	2.455	431	440	448	rBV2	6930	10664	2.20%	0.244%
7	3.812	849	862	893	rBV2	41529	154360	31.89%	3.533%
8	4.259	983	1001	1040	rBV3	94301	275552	56.93%	6.307%
9	4.966	1202	1221	1248	rBV3	187142	483977	100.00%	11.078%
10	5.542	1386	1400	1425	rBV	189786	394036	81.42%	9.020%
11	5.995	1528	1541	1574	rBV	114891	239514	49.49%	5.483%
12	6.921	1816	1829	1845	rBV	46773	86236	17.82%	1.974%
13	7.249	1919	1931	1949	rBV	217641	386450	79.85%	8.846%
14	7.561	2018	2028	2053	rBV2	28049	50811	10.50%	1.163%
15	7.883	2116	2128	2141	rBV2	3654	6491	1.34%	0.149%
16	8.034	2163	2175	2212	rBV	212073	397912	82.22%	9.108%
17	8.793	2399	2411	2438	rBV	292838	481693	99.53%	11.026%
18	10.162	2826	2837	2859	rBV	88065	140697	29.07%	3.221%
19	10.333	2879	2890	2904	rVB	8682	14188	2.93%	0.325%
20	11.194	3145	3158	3181	rBV	304731	478581	98.89%	10.955%
21	11.571	3263	3275	3294	rBV	226636	363423	75.09%	8.319%
22	12.204	3461	3472	3484	rVB3	4558	7220	1.49%	0.165%
23	12.297	3490	3501	3509	rVB4	5231	7213	1.49%	0.165%




Sum of corrected areas: 4368658

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030114.D
Acq On : 02 Mar 2023 11:54
Operator : SY/MD
Sample : 01729-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BY9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

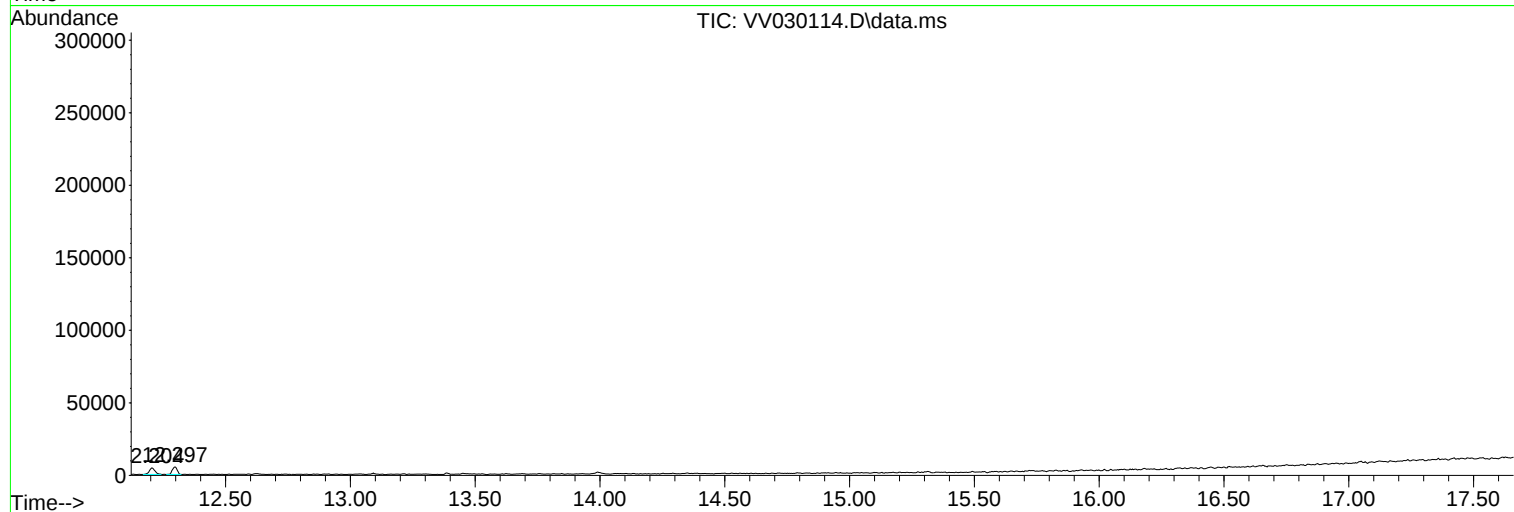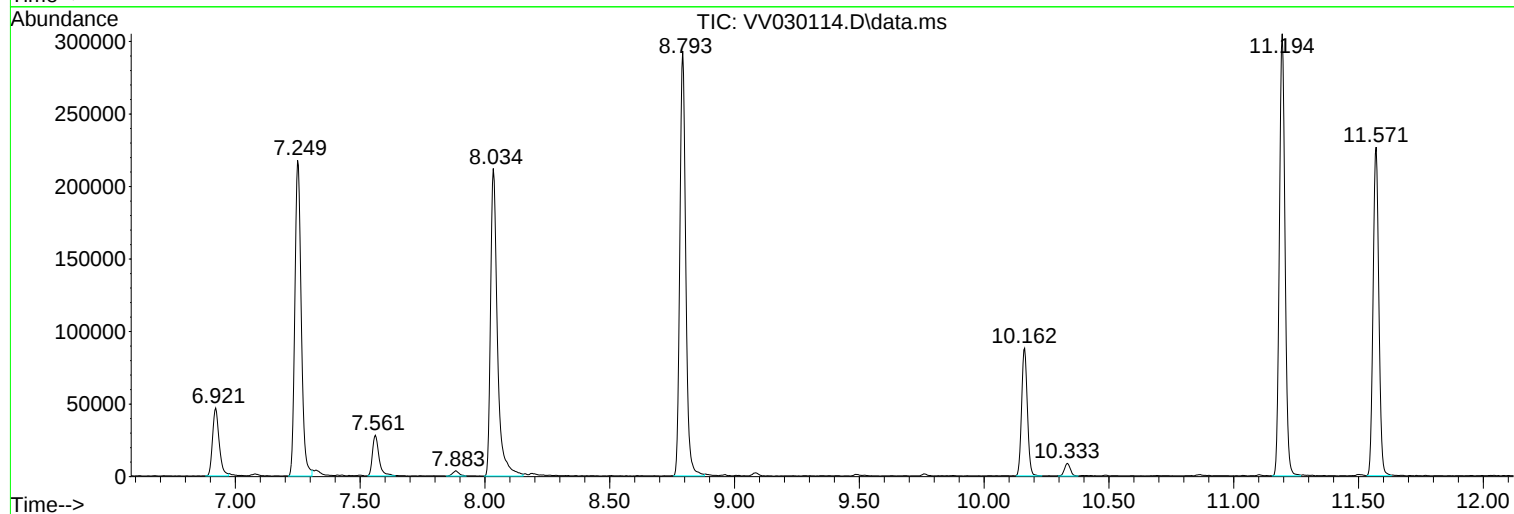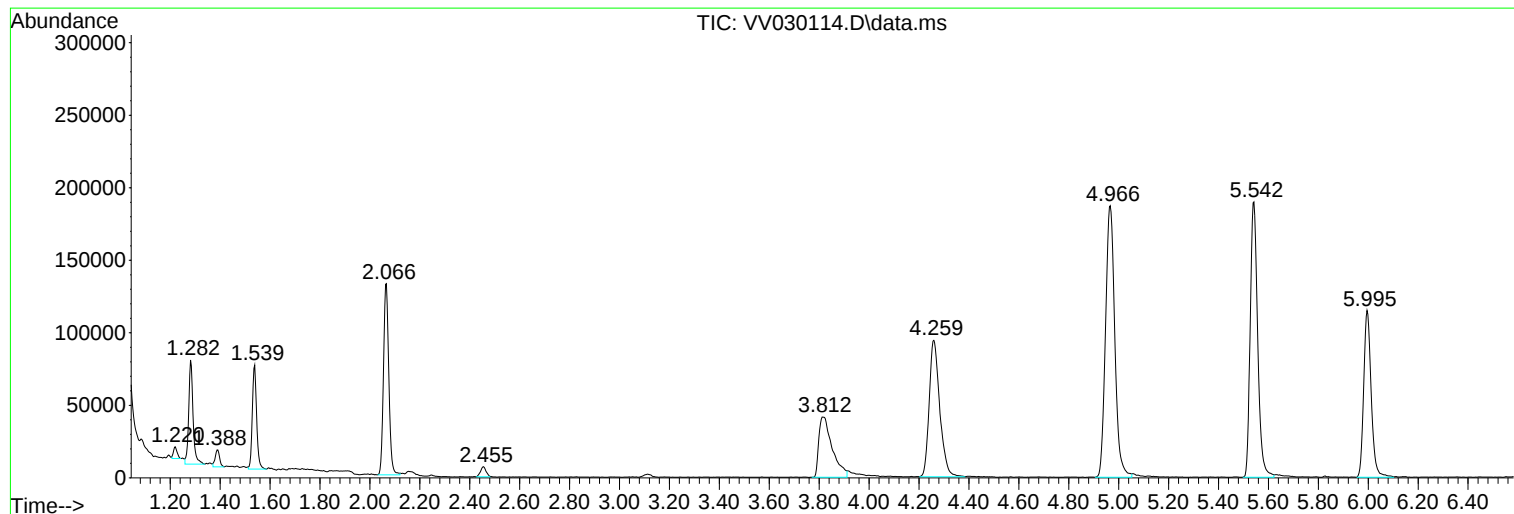

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030114.D
Acq On : 02 Mar 2023 11:54
Operator : SY/MD
Sample : 01729-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BY9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030114.D
Acq On : 02 Mar 2023 11:54
Operator : SY/MD
Sample : 01729-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BY9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc