

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
 Data File : VV030115.D
 Acq On : 02 Mar 2023 12:18
 Operator : SY/MD
 Sample : 01729-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BZ9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030115.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	51	56	60	rBV	5006	5275	1.12%	0.128%
2	1.282	69	75	85	rVB	63033	64968	13.77%	1.571%
3	1.539	148	155	166	rVB	67900	77977	16.53%	1.886%
4	2.066	305	319	337	rBV	128397	187477	39.74%	4.534%
5	3.818	850	864	901	rBV	41399	153775	32.59%	3.719%
6	4.262	985	1002	1032	rBV2	90817	249923	52.97%	6.044%
7	4.969	1204	1222	1251	rBV2	184908	471816	100.00%	11.410%
8	5.545	1387	1401	1427	rBV	174531	363481	77.04%	8.790%
9	5.998	1528	1542	1563	rBV	111832	230832	48.92%	5.582%
10	6.921	1818	1829	1856	rBV	44544	84858	17.99%	2.052%
11	7.252	1920	1932	1959	rBV	212346	378753	80.28%	9.159%
12	7.561	2019	2028	2052	rBV2	26737	49089	10.40%	1.187%
13	7.886	2117	2129	2145	rVB2	6007	10348	2.19%	0.250%
14	8.034	2164	2175	2209	rBV	206860	388305	82.30%	9.390%
15	8.792	2395	2411	2446	rBV	265057	444279	94.16%	10.744%
16	10.162	2826	2837	2857	rBV	88270	140321	29.74%	3.393%
17	10.336	2879	2891	2905	rVB	17085	27056	5.73%	0.654%
18	11.194	3147	3158	3180	rBV	286025	438603	92.96%	10.607%
19	11.571	3263	3275	3291	rBV	223700	352978	74.81%	8.536%
20	12.207	3463	3473	3483	rVB2	6295	10064	2.13%	0.243%
21	13.995	4018	4029	4039	rBV2	2905	4936	1.05%	0.119%




Sum of corrected areas: 4135114

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030115.D
Acq On : 02 Mar 2023 12:18
Operator : SY/MD
Sample : 01729-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BZ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

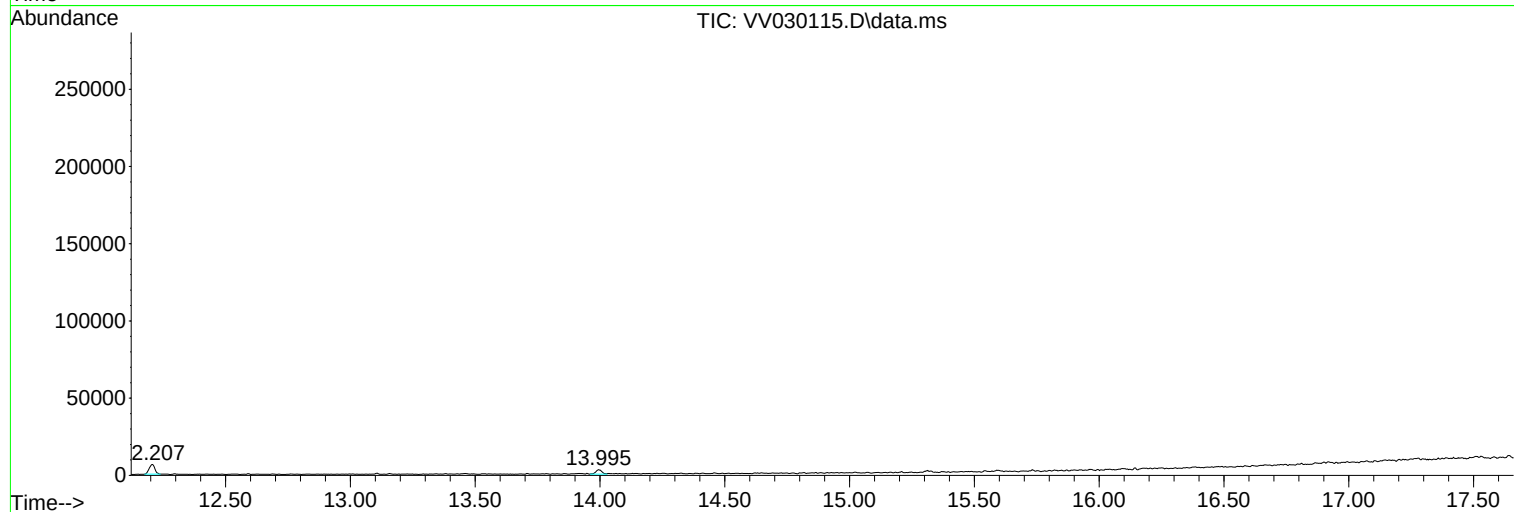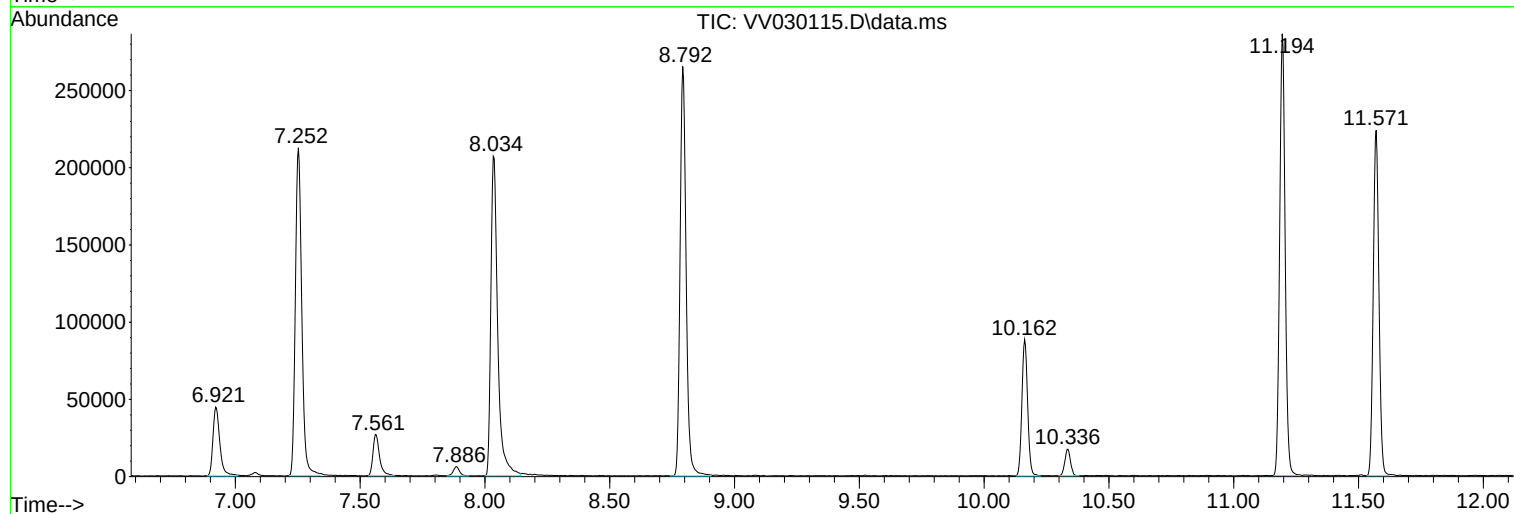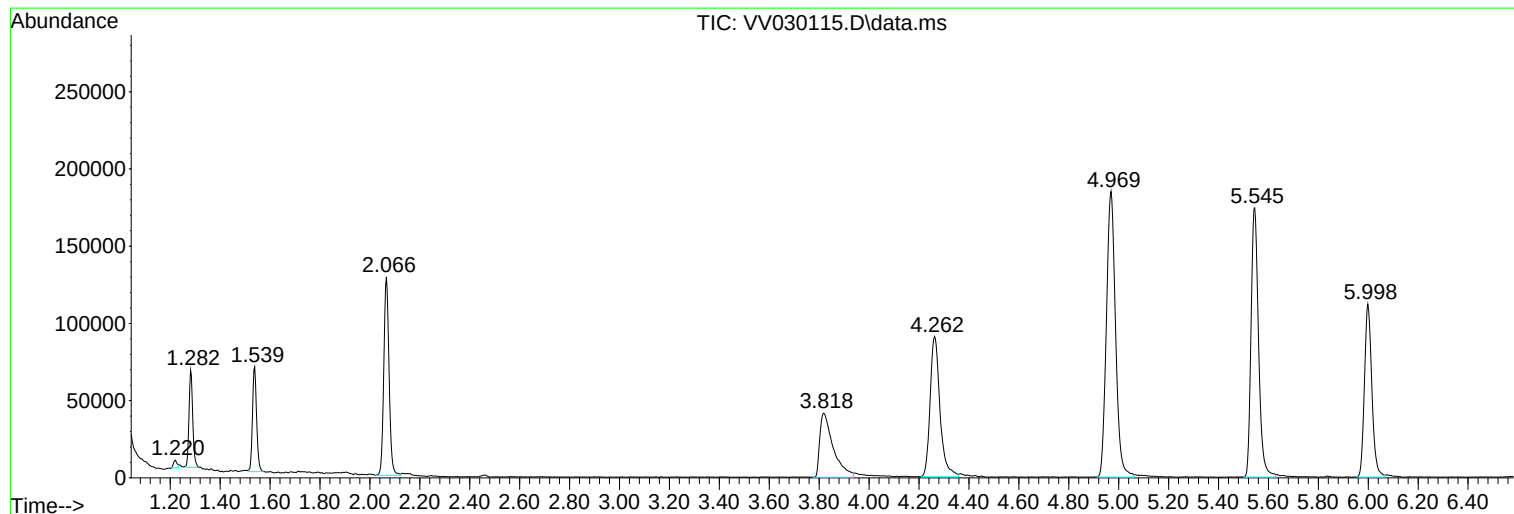

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030115.D
Acq On : 02 Mar 2023 12:18
Operator : SY/MD
Sample : 01729-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BZ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030115.D
Acq On : 02 Mar 2023 12:18
Operator : SY/MD
Sample : 01729-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BZ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------