

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
 Data File : VV030116.D
 Acq On : 02 Mar 2023 12:43
 Operator : SY/MD
 Sample : 01729-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030116.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	51	56	64	rBV2	4864	6343	1.31%	0.156%
2	1.282	69	75	86	rVB	66271	68556	14.18%	1.684%
3	1.539	147	155	167	rVB	69890	82756	17.12%	2.033%
4	2.066	308	319	334	rBV	132527	193486	40.03%	4.752%
5	2.455	431	440	452	rBV2	5660	9551	1.98%	0.235%
6	3.822	852	865	904	rBV	44657	170165	35.20%	4.180%
7	4.262	985	1002	1027	rBV2	90258	225550	46.66%	5.540%
8	4.970	1205	1222	1247	rBV2	191440	483397	100.00%	11.873%
9	5.545	1387	1401	1427	rBV	154420	320691	66.34%	7.877%
10	5.998	1526	1542	1566	rBV	114115	239679	49.58%	5.887%
11	6.924	1817	1830	1846	rBV	45131	84589	17.50%	2.078%
12	7.252	1920	1932	1967	rBV	217495	389910	80.66%	9.577%
13	7.564	2018	2029	2050	rBV	28342	50535	10.45%	1.241%
14	7.886	2117	2129	2142	rVB3	3941	7589	1.57%	0.186%
15	8.037	2165	2176	2213	rBV	207595	398863	82.51%	9.797%
16	8.371	2270	2280	2297	rVB	8038	14090	2.91%	0.346%
17	8.793	2400	2411	2440	rBV	241008	401707	83.10%	9.867%
18	10.162	2826	2837	2857	rBV	91508	144482	29.89%	3.549%
19	10.333	2879	2890	2901	rBV2	10117	16694	3.45%	0.410%
20	11.194	3147	3158	3180	rBV	254765	390937	80.87%	9.602%
21	11.571	3262	3275	3295	rBV	231508	361163	74.71%	8.871%
22	12.204	3462	3472	3483	rVB2	6813	10533	2.18%	0.259%




Sum of corrected areas: 4071266

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030116.D
Acq On : 02 Mar 2023 12:43
Operator : SY/MD
Sample : 01729-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

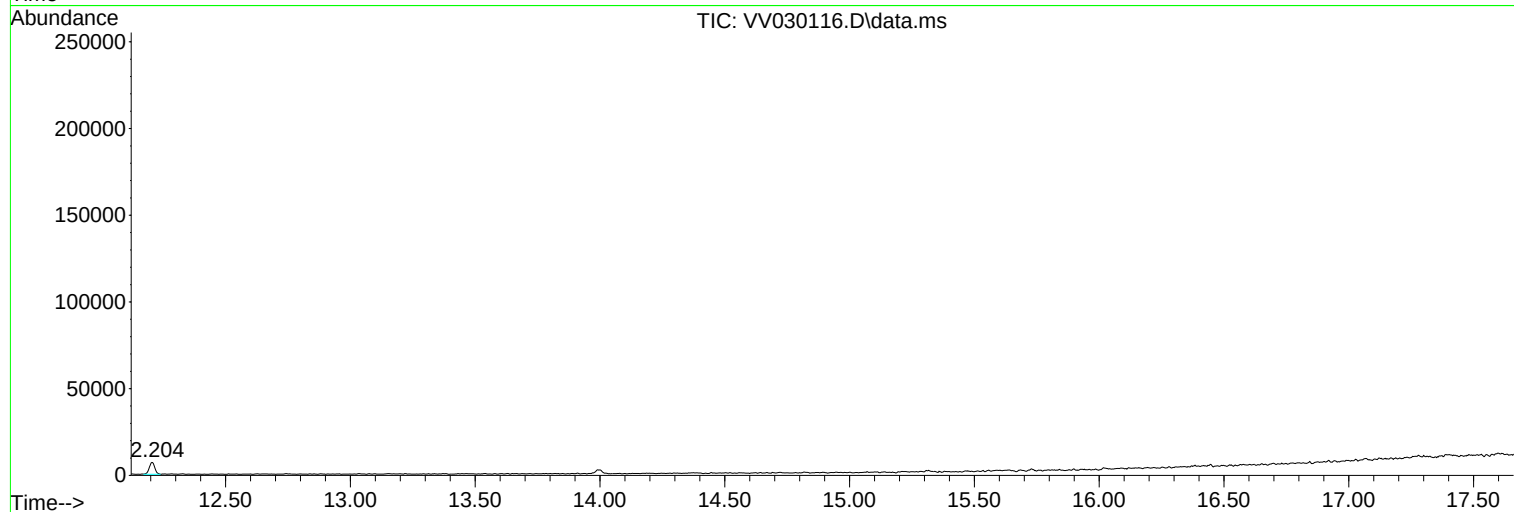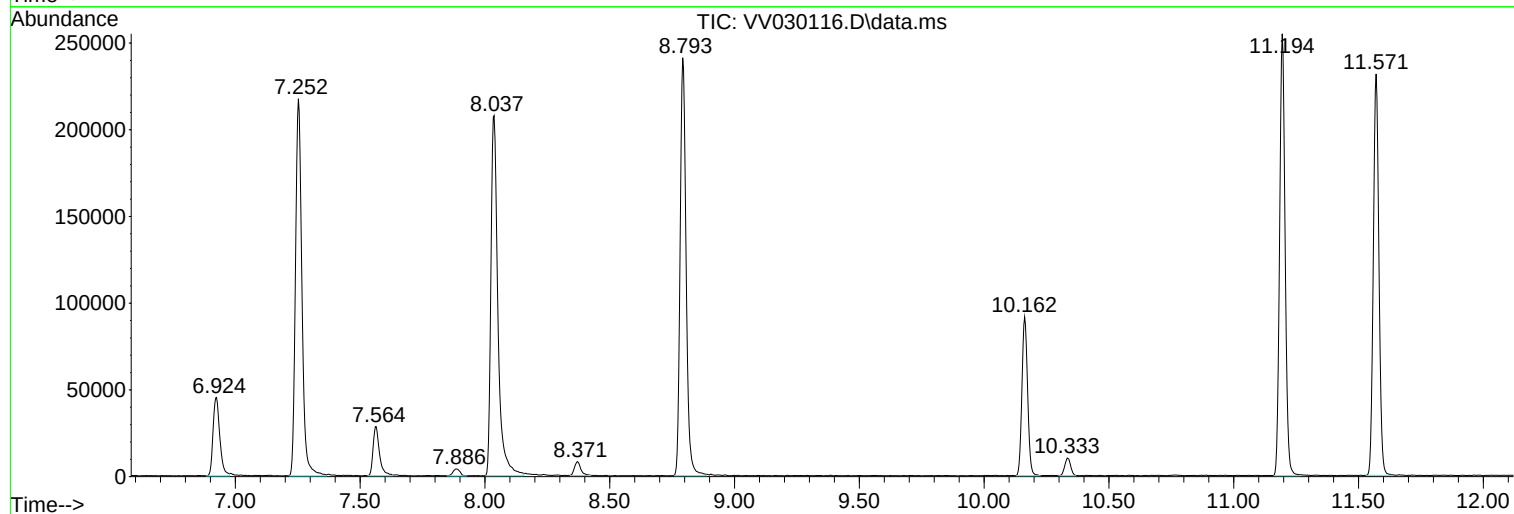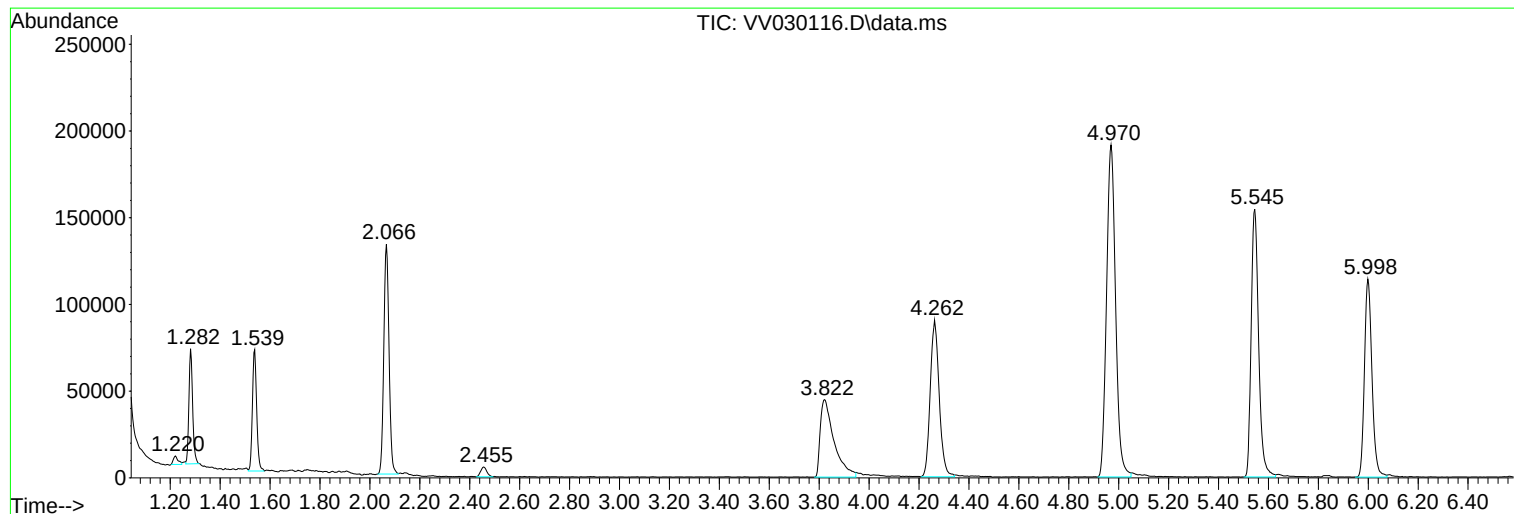

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030116.D
Acq On : 02 Mar 2023 12:43
Operator : SY/MD
Sample : 01729-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030116.D
Acq On : 02 Mar 2023 12:43
Operator : SY/MD
Sample : 01729-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------