

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
 Data File : VV030117.D
 Acq On : 02 Mar 2023 13:05
 Operator : SY/MD
 Sample : 01769-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBYL6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030117.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	90	rVB	69950	79205	15.94%	1.680%
2	1.539	147	155	169	rVB	70673	85304	17.16%	1.809%
3	2.066	307	319	332	rBV	135180	197924	39.82%	4.198%
4	2.150	333	345	370	rVB2	20516	67697	13.62%	1.436%
5	2.407	376	425	429	rBV2	81503	451716	90.89%	9.581%
6	3.821	854	865	920	rBV	42870	175492	35.31%	3.722%
7	4.265	985	1003	1028	rBV2	91196	232388	46.76%	4.929%
8	4.969	1205	1222	1258	rBV2	194065	496986	100.00%	10.541%
9	5.545	1385	1401	1432	rBV	161411	338422	68.09%	7.178%
10	6.001	1528	1543	1564	rBV	116964	245190	49.34%	5.201%
11	6.924	1816	1830	1852	rBV	46906	89146	17.94%	1.891%
12	7.252	1919	1932	1948	rBV	222473	393783	79.23%	8.352%
13	7.329	1949	1956	1974	rVB	12290	22743	4.58%	0.482%
14	7.564	2020	2029	2046	rBV2	28970	51293	10.32%	1.088%
15	8.037	2165	2176	2213	rBV	226602	425811	85.68%	9.032%
16	8.796	2399	2412	2438	rBV	247106	417441	83.99%	8.854%
17	10.162	2826	2837	2858	rVB	95315	148858	29.95%	3.157%
18	10.332	2880	2890	2900	rVB3	5166	8562	1.72%	0.182%
19	11.194	3147	3158	3182	rBV	263901	408255	82.15%	8.659%
20	11.500	3244	3253	3264	rBV4	2950	5678	1.14%	0.120%
21	11.570	3264	3275	3296	rVB	242578	372802	75.01%	7.907%




Sum of corrected areas: 4714696

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030117.D
Acq On : 02 Mar 2023 13:05
Operator : SY/MD
Sample : 01769-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBYL6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

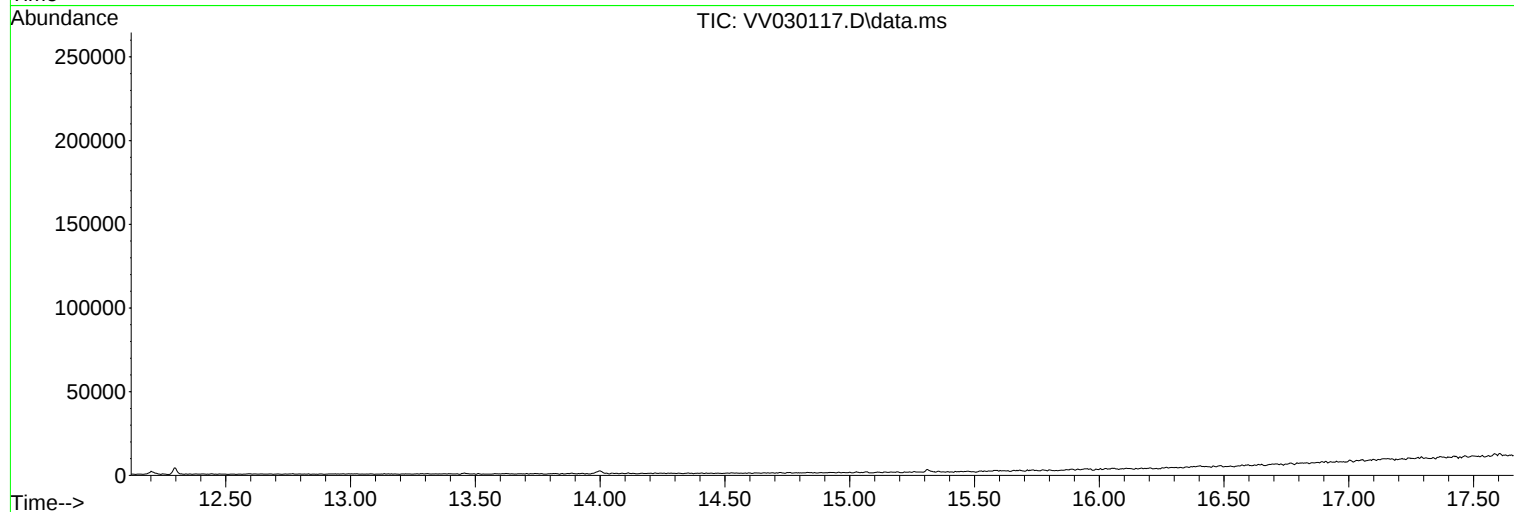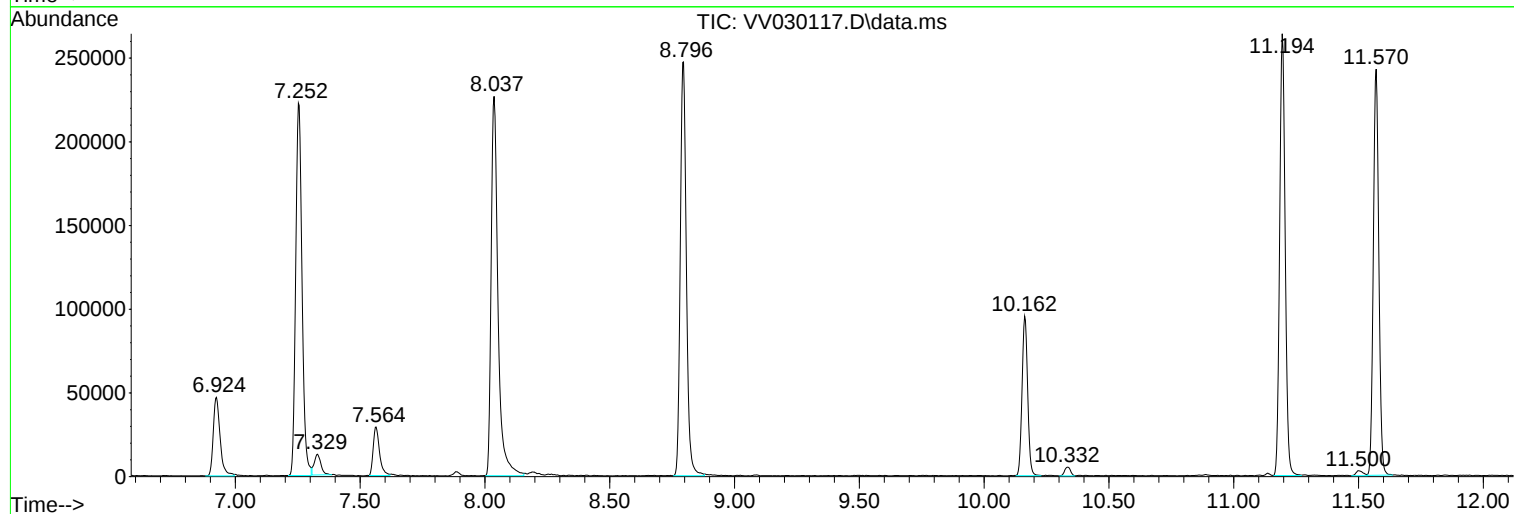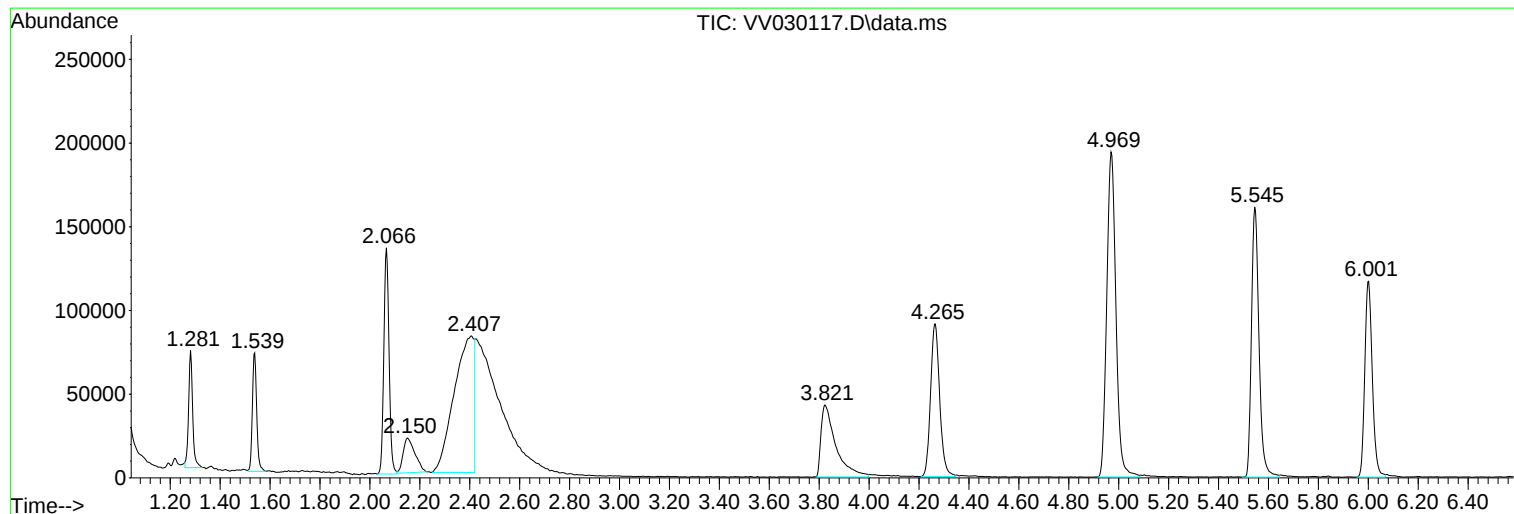

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030117.D
Acq On : 02 Mar 2023 13:05
Operator : SY/MD
Sample : 01769-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBYL6










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.407	6.67 ug/L	451716	1,4-Difluorobenzene	5.545

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Isopropyl Alcohol			60	C3H8O	000067-63-0	83
2	Isopropyl Alcohol			60	C3H8O	000067-63-0	78
3	Isopropyl Alcohol			60	C3H8O	000067-63-0	78
4	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
5	Isopropyl Alcohol			60	C3H8O	000067-63-0	64

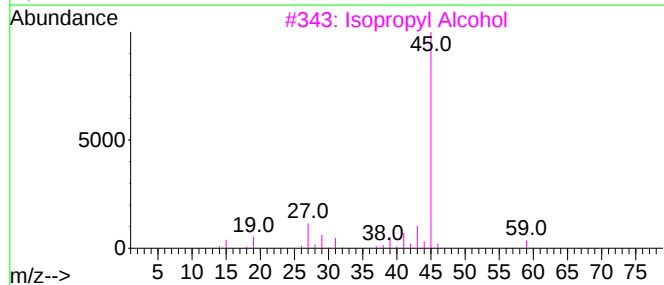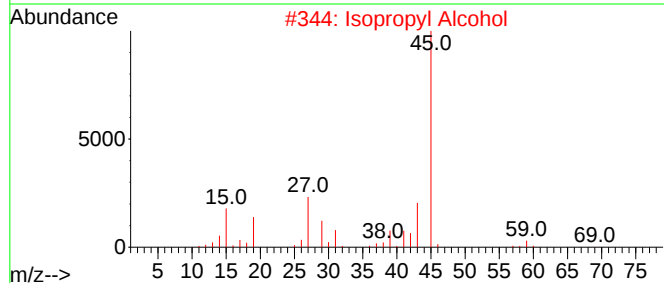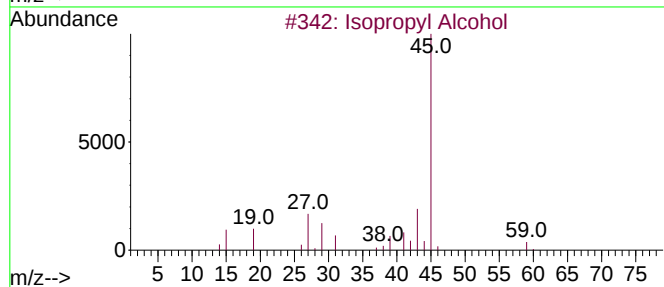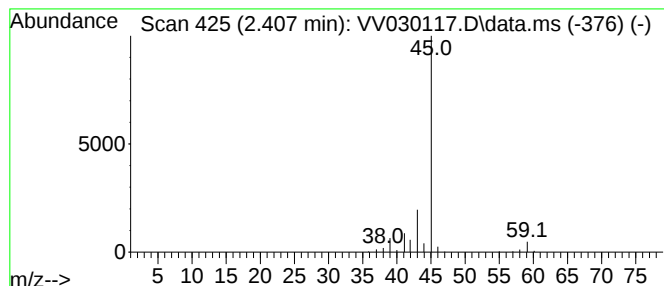

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030117.D
Acq On : 02 Mar 2023 13:05
Operator : SY/MD
Sample : 01769-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBYL6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.407	6.7	ug/L	451716	1	5.545	338422	5.0