

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
 Data File : VV030123.D
 Acq On : 02 Mar 2023 17:23
 Operator : SY/MD
 Sample : 01769-03 500X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBYL3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030123.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	60	rBV2	5496	6532	1.43%	0.168%
2	1.282	69	75	91	rVB	59206	66015	14.50%	1.695%
3	1.536	146	154	172	rVB	64655	79625	17.48%	2.044%
4	2.066	302	319	334	rBV	122400	179799	39.48%	4.616%
5	2.455	431	440	453	rVB2	12561	20921	4.59%	0.537%
6	3.828	854	867	906	rBV2	37123	150850	33.12%	3.873%
7	4.262	984	1002	1028	rBV	82659	210830	46.30%	5.412%
8	4.969	1205	1222	1249	rBV2	177270	455404	100.00%	11.691%
9	5.545	1387	1401	1420	rBV	154031	319194	70.09%	8.194%
10	5.998	1526	1542	1565	rBV	106834	223255	49.02%	5.731%
11	6.924	1819	1830	1857	rBV	42981	81517	17.90%	2.093%
12	7.252	1920	1932	1968	rBV	202271	366491	80.48%	9.408%
13	7.564	2018	2029	2047	rBV	25740	47097	10.34%	1.209%
14	8.037	2162	2176	2210	rBV	203589	397129	87.20%	10.195%
15	8.371	2269	2280	2291	rVB2	3358	5050	1.11%	0.130%
16	8.792	2399	2411	2436	rBV	234869	397383	87.26%	10.201%
17	10.162	2825	2837	2859	rVB	89436	136638	30.00%	3.508%
18	11.194	3147	3158	3179	rBV	244596	380711	83.60%	9.773%
19	11.570	3260	3275	3292	rBV	211016	338397	74.31%	8.687%
20	12.201	3463	3471	3485	rVB3	4654	7208	1.58%	0.185%
21	12.593	3586	3593	3605	rVB3	3856	5582	1.23%	0.143%
22	13.689	3925	3934	3945	rBV4	13488	19774	4.34%	0.508%




Sum of corrected areas: 3895402

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030123.D
Acq On : 02 Mar 2023 17:23
Operator : SY/MD
Sample : 01769-03 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBYL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

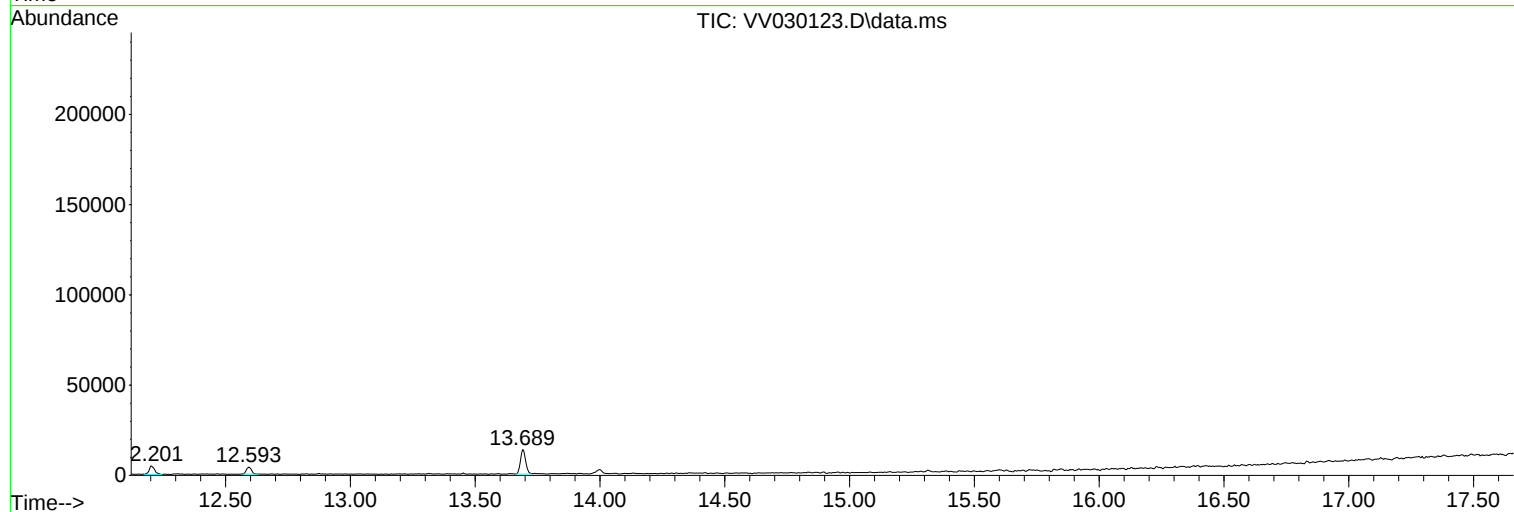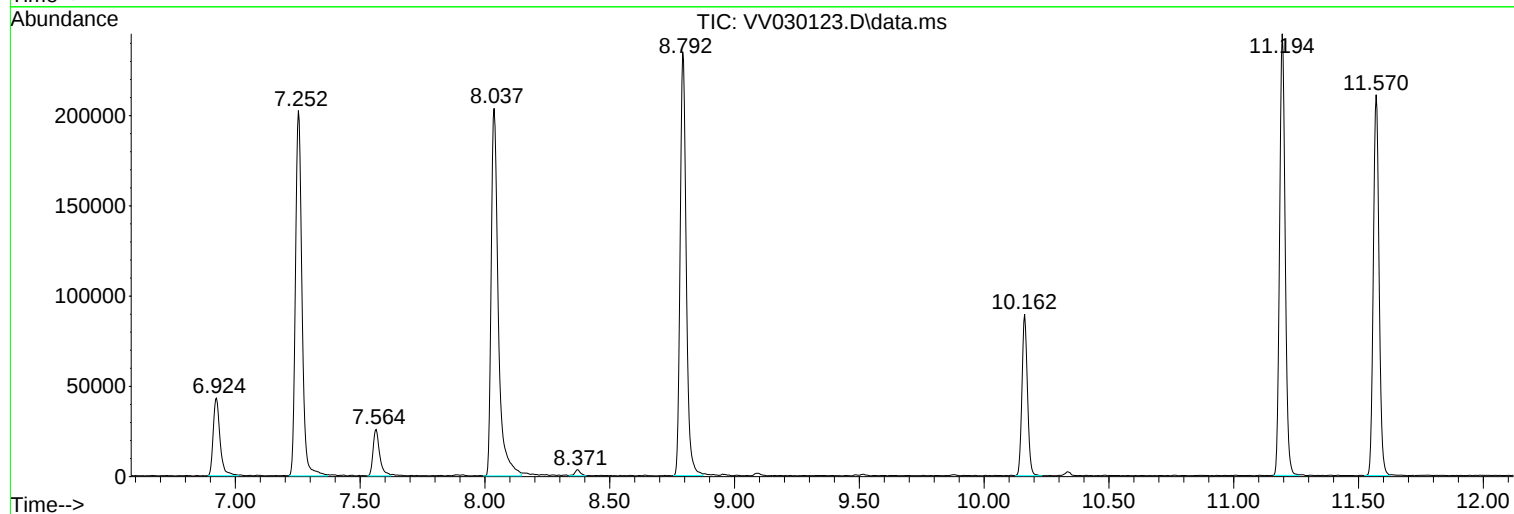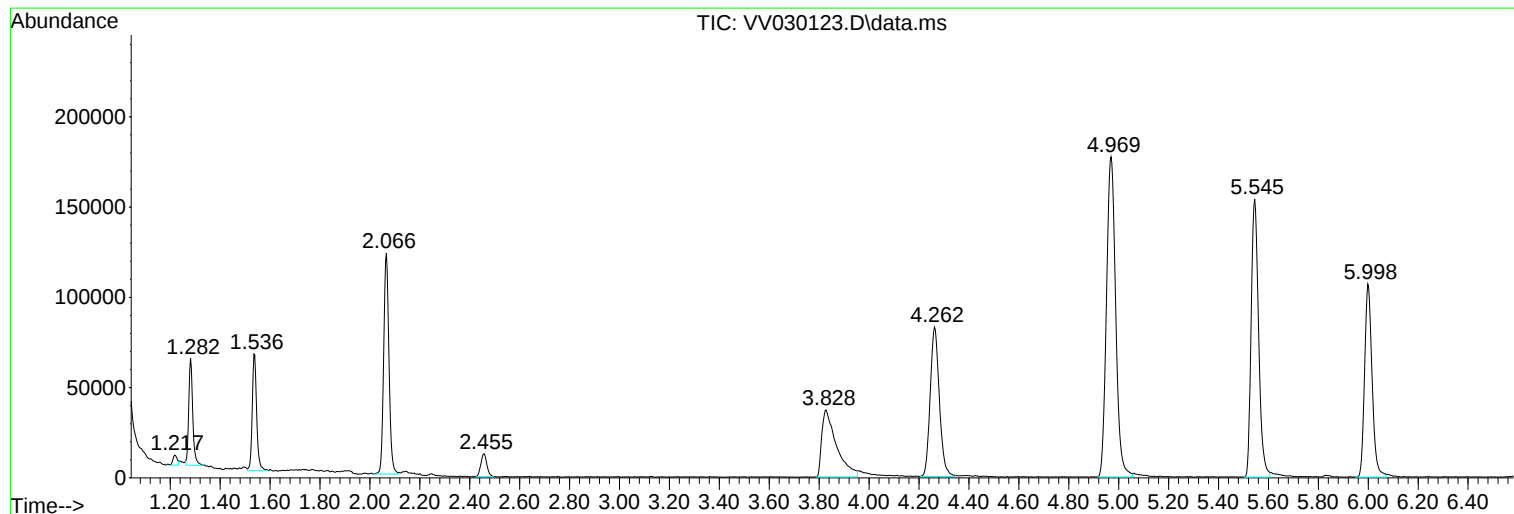

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030123.D
Acq On : 02 Mar 2023 17:23
Operator : SY/MD
Sample : 01769-03 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBYL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030123.D
Acq On : 02 Mar 2023 17:23
Operator : SY/MD
Sample : 01769-03 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBYL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------