

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
 Data File : VV030124.D
 Acq On : 02 Mar 2023 17:47
 Operator : SY/MD
 Sample : 01769-04 500X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBYL4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030124.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	51	56	62	rBV2	4824	5809	1.32%	0.159%
2	1.281	69	75	91	rVB	60952	66701	15.16%	1.825%
3	1.535	147	154	165	rVB	61986	72185	16.41%	1.975%
4	2.063	306	318	333	rBV	119073	175304	39.84%	4.795%
5	2.455	428	440	456	rBV3	10199	17310	3.93%	0.474%
6	3.838	859	870	872	rBV2	24022	36461	8.29%	0.997%
7	4.262	984	1002	1030	rBV2	79686	205033	46.60%	5.609%
8	4.969	1204	1222	1253	rBV2	171743	439980	100.00%	12.036%
9	5.545	1385	1401	1421	rBV	154885	318011	72.28%	8.699%
10	5.998	1524	1542	1569	rBV	104292	219675	49.93%	6.009%
11	6.924	1817	1830	1854	rBV	41739	79606	18.09%	2.178%
12	7.252	1920	1932	1953	rBV	195851	348151	79.13%	9.524%
13	7.564	2018	2029	2058	rBV2	23842	45752	10.40%	1.252%
14	8.040	2165	2177	2211	rBV	184138	381413	86.69%	10.434%
15	8.371	2270	2280	2292	rVB4	2756	4474	1.02%	0.122%
16	8.792	2399	2411	2438	rBV	232927	393804	89.50%	10.773%
17	10.162	2825	2837	2863	rVB	83767	134543	30.58%	3.680%
18	11.194	3144	3158	3179	rBV	245815	378023	85.92%	10.341%
19	11.570	3263	3275	3298	rBV	204765	320476	72.84%	8.767%
20	12.204	3460	3472	3481	rVB3	4733	7099	1.61%	0.194%
21	13.995	4016	4029	4041	rBV	3215	5790	1.32%	0.158%




Sum of corrected areas: 3655600

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030124.D
Acq On : 02 Mar 2023 17:47
Operator : SY/MD
Sample : 01769-04 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBYL4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

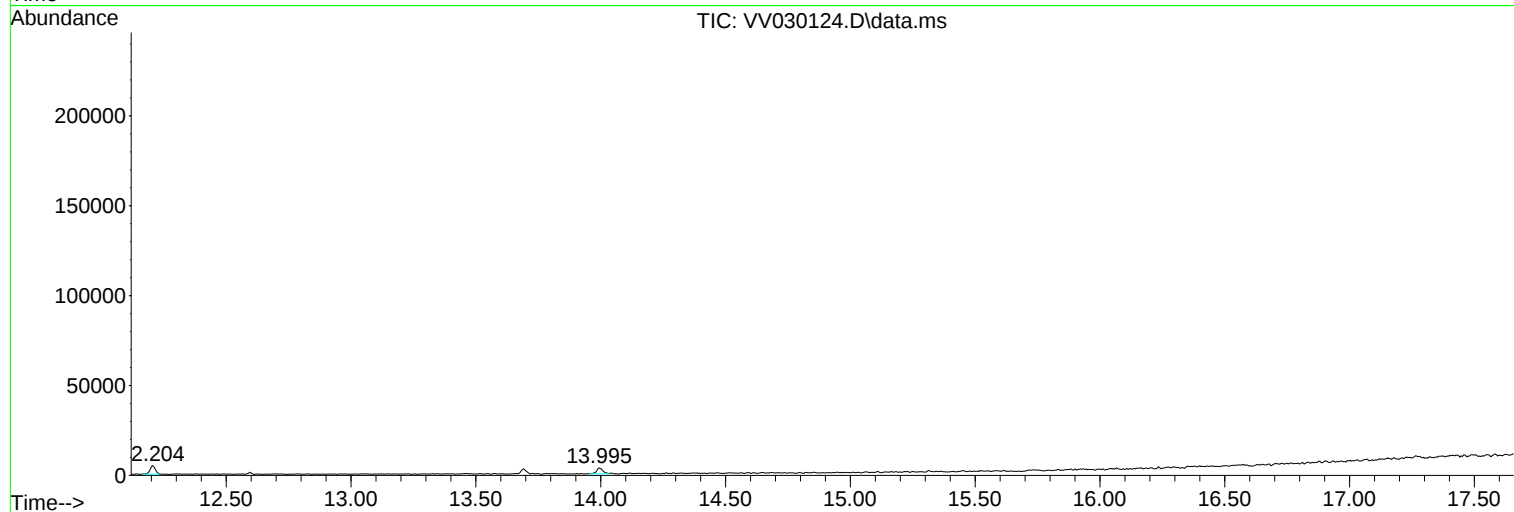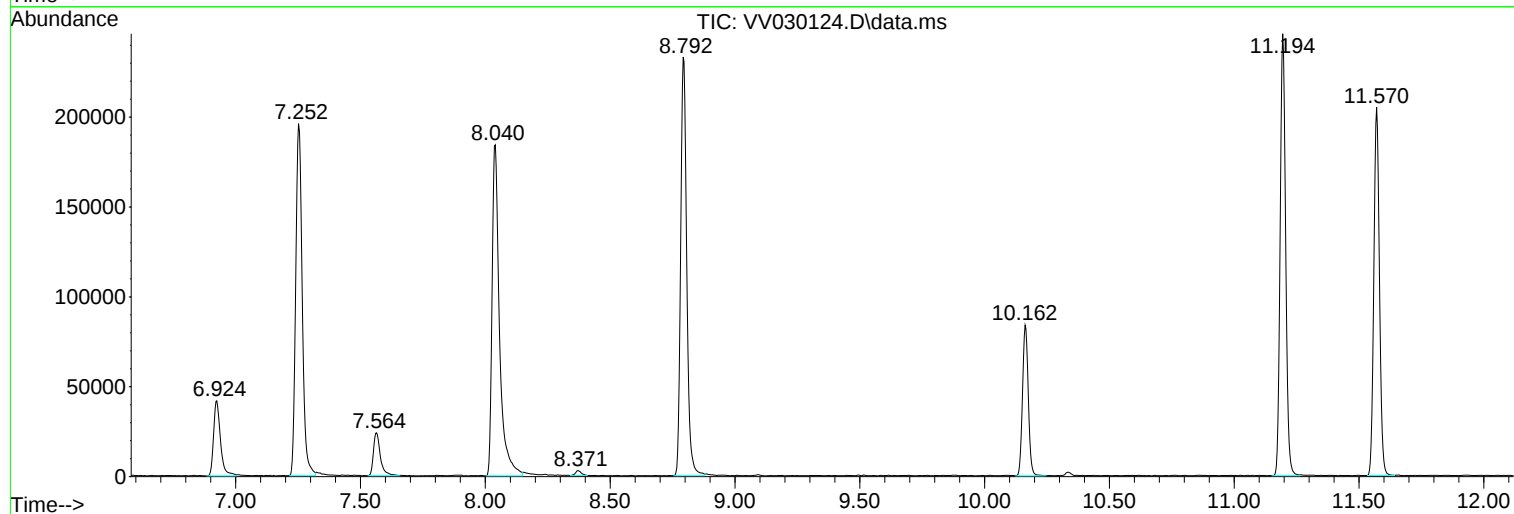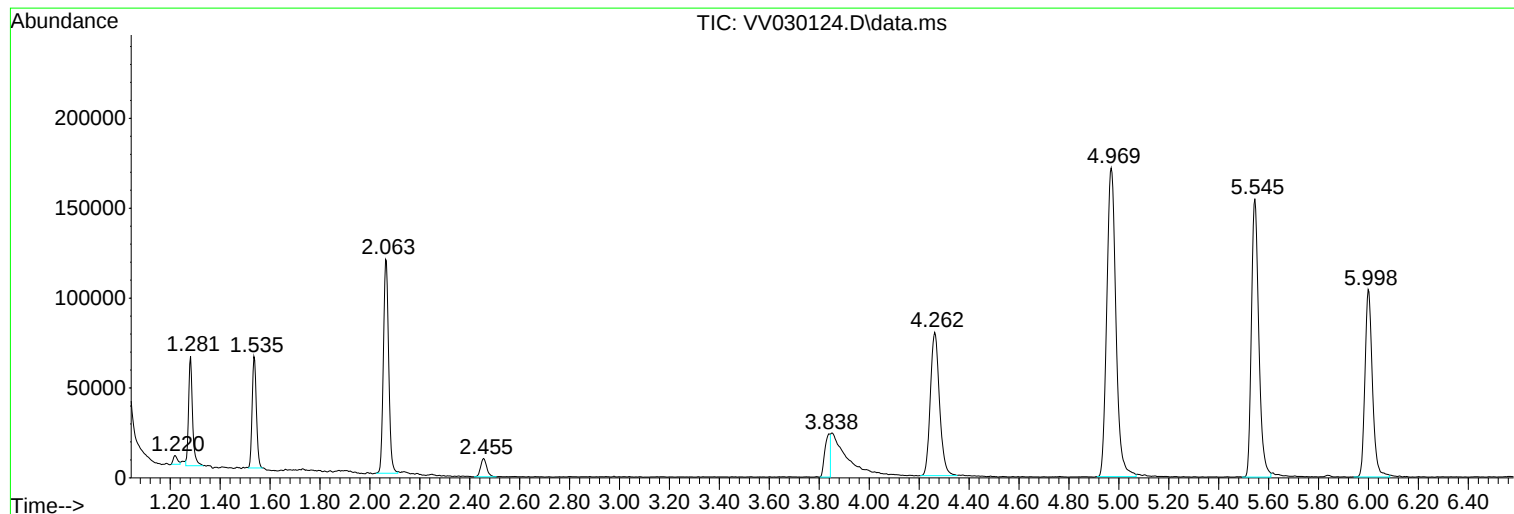

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030124.D
Acq On : 02 Mar 2023 17:47
Operator : SY/MD
Sample : 01769-04 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBYL4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030124.D
Acq On : 02 Mar 2023 17:47
Operator : SY/MD
Sample : 01769-04 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBYL4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc