

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
 Data File : VV030125.D
 Acq On : 02 Mar 2023 18:11
 Operator : SY/MD
 Sample : 01769-05 500X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBYL5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030125.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	98	rVB	58976	70110	15.94%	1.886%
2	1.535	147	154	166	rVB	61996	73290	16.66%	1.972%
3	2.063	307	318	331	rBV	120130	173922	39.54%	4.679%
4	2.455	431	440	451	rBV	15477	24994	5.68%	0.672%
5	3.841	858	871	905	rBV	24375	124393	28.28%	3.347%
6	4.262	983	1002	1030	rBV2	80249	208789	47.47%	5.617%
7	4.969	1206	1222	1252	rBV2	174257	439851	100.00%	11.834%
8	5.545	1387	1401	1427	rBV	150661	314202	71.43%	8.454%
9	5.998	1528	1542	1570	rBV	104274	218592	49.70%	5.881%
10	6.924	1819	1830	1859	rBV	40172	77875	17.70%	2.095%
11	7.252	1919	1932	1959	rBV	192665	345127	78.46%	9.286%
12	7.564	2018	2029	2050	rBV	24139	44564	10.13%	1.199%
13	8.037	2161	2176	2219	rBV	179490	377799	85.89%	10.165%
14	8.792	2397	2411	2439	rBV	236225	389315	88.51%	10.474%
15	10.162	2826	2837	2858	rVB	84487	134041	30.47%	3.606%
16	11.194	3146	3158	3184	rBV	236268	371624	84.49%	9.998%
17	11.570	3263	3275	3293	rBV	202300	315916	71.82%	8.500%
18	12.201	3462	3471	3482	rBV3	4095	7376	1.68%	0.198%
19	13.998	4020	4030	4042	rVB	2682	5035	1.14%	0.135%




Sum of corrected areas: 3716815

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030125.D
Acq On : 02 Mar 2023 18:11
Operator : SY/MD
Sample : 01769-05 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBYL5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

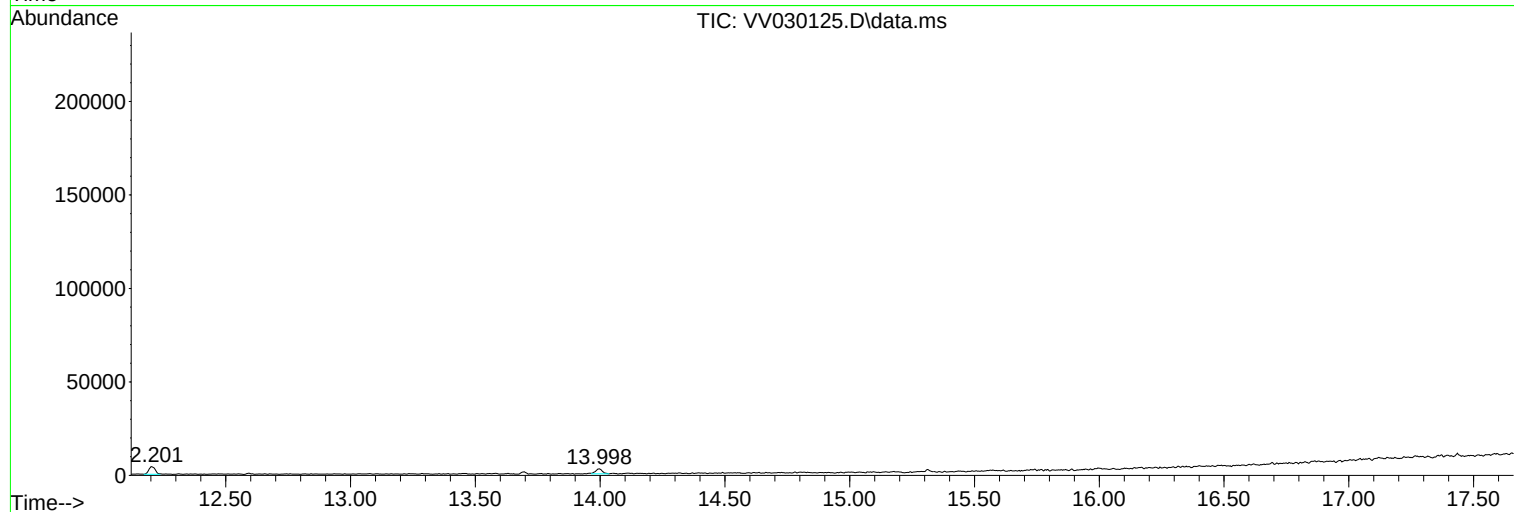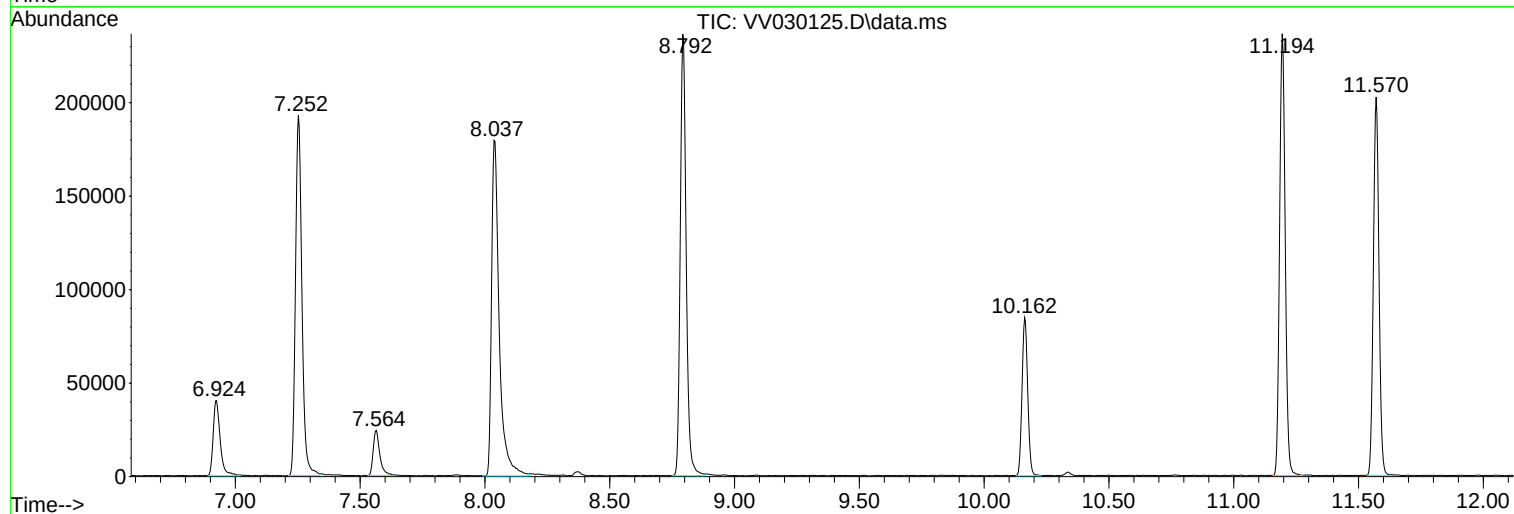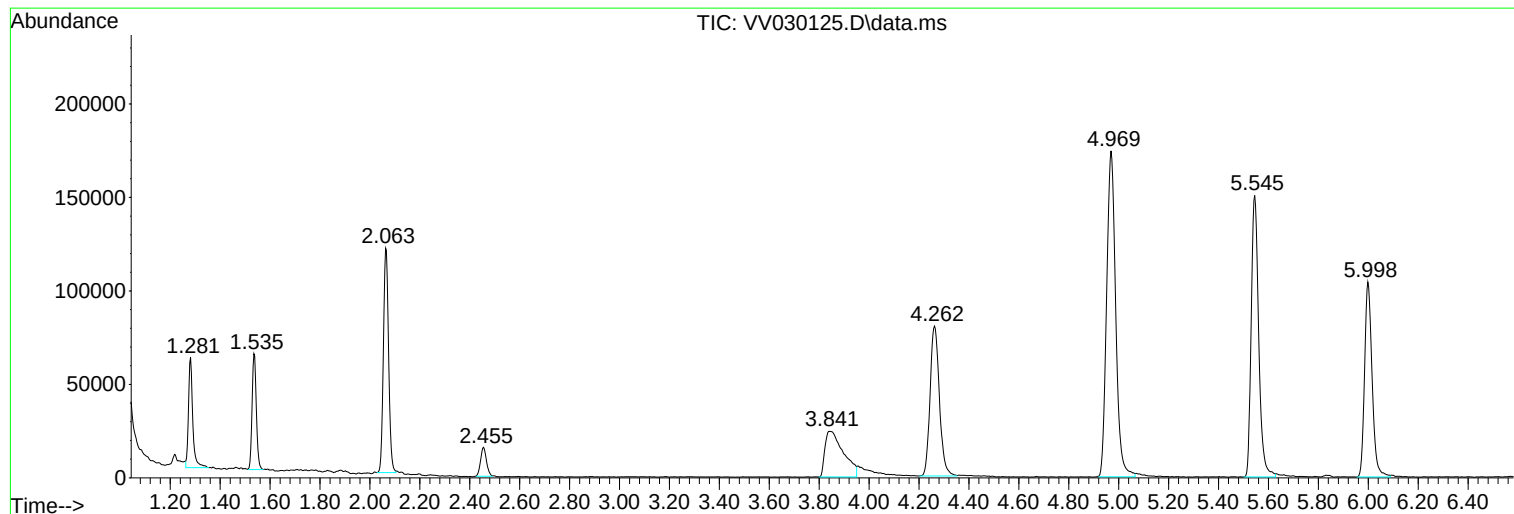

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030125.D
Acq On : 02 Mar 2023 18:11
Operator : SY/MD
Sample : 01769-05 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBYL5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030125.D
Acq On : 02 Mar 2023 18:11
Operator : SY/MD
Sample : 01769-05 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBYL5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc