
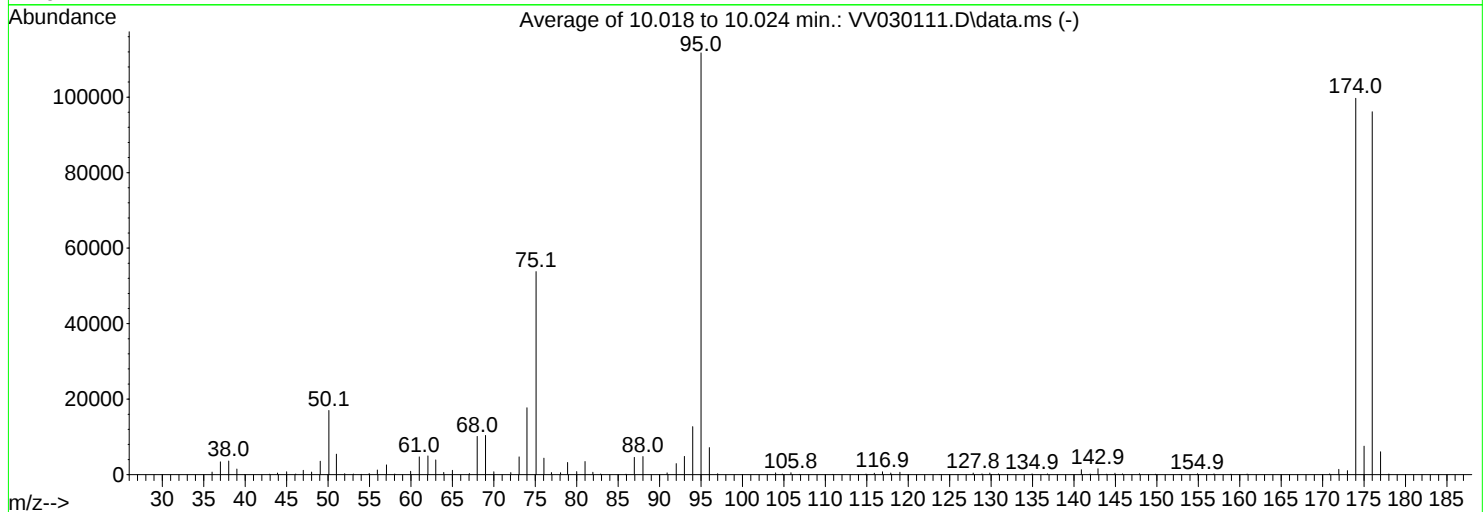


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030223\
Data File : VV030111.D
Acq On : 02 Mar 2023 09:12
Operator : SY/MD
Sample : BFB226
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB226

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Mar 03 03:28:37 2023

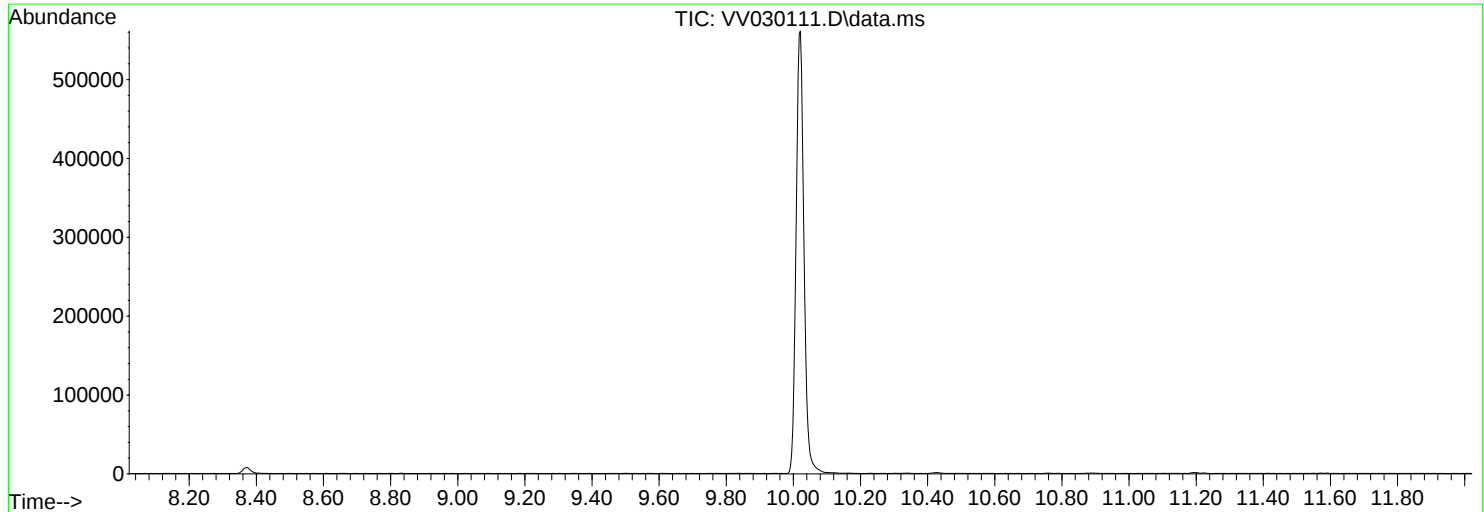

AutoFind: Scans 2792, 2793, 2794; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	17013	PASS
75	95	30	80	48.1	53768	PASS
95	95	100	100	100.0	111739	PASS
96	95	5	9	6.4	7176	PASS
173	174	0.00	2	1.1	1082	PASS
174	95	50	120	89.2	99699	PASS
175	174	5	9	7.6	7546	PASS
176	174	95	105	96.4	96112	PASS
177	176	5	10	6.3	6068	PASS

m/z	Abundance
39.90	204.0
43.90	320.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226

m/z	Abundance
36.00	701.0
37.00	3609.0
38.00	3731.0
39.00	1501.0
39.90	250.0
43.00	117.0
44.00	797.0
45.00	835.0
46.10	165.0
47.00	1129.0
48.00	669.0
49.00	3851.0
50.10	18056.0
51.00	5789.0
52.00	284.0
53.00	169.0
55.00	296.0
56.00	1275.0
57.10	2607.0
58.10	160.0
59.90	950.0
61.00	4777.0
62.00	4964.0
63.00	4065.0
64.00	660.0
65.00	1246.0
67.00	298.0
68.00	10684.0
69.00	10871.0
70.00	819.0
72.00	599.0
73.00	4935.0
74.00	18264.0
75.10	55848.0
76.00	4494.0
76.90	544.0
78.00	566.0
78.90	3259.0
80.00	835.0
81.00	3595.0
81.90	641.0
82.90	121.0
85.90	175.0
87.00	4855.0
88.00	4966.0
90.90	466.0
92.00	3084.0
93.00	4818.0
94.00	13075.0
95.00	114920.0
96.00	7690.0
97.00	270.0
104.00	453.0
104.80	228.0
105.80	515.0
106.90	108.0
114.90	138.0
115.90	395.0
116.90	725.0
117.90	401.0
119.00	651.0
123.80	113.0
127.90	470.0
128.90	228.0
129.90	408.0
130.90	219.0
135.00	212.0
136.80	201.0
140.90	1353.0
142.00	190.0
142.90	1660.0
144.00	124.0
144.90	440.0
145.80	216.0
147.90	257.0
149.80	155.0
154.90	284.0
156.90	237.0
159.00	143.0
160.90	180.0
170.90	205.0
172.00	1379.0
173.00	1139.0
174.00	100504.0
175.00	7815.0
176.00	96688.0
177.00	6253.0
178.00	213.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226

m/z	Abundance
36.00	704.0
37.00	3435.0
38.00	3763.0
39.00	1477.0
39.90	256.0
42.90	122.0
44.00	768.0
45.00	787.0
46.10	172.0
47.00	1189.0
48.00	706.0
49.00	3684.0
50.10	17488.0
51.00	5665.0
52.00	250.0
53.10	170.0
54.00	105.0
55.00	320.0
56.00	1284.0
57.00	2698.0
58.00	166.0
59.90	877.0
61.00	4866.0
62.10	5139.0
63.00	4041.0
64.00	585.0
65.00	1167.0
67.10	293.0
68.00	10455.0
69.00	10657.0
70.00	771.0
72.00	563.0
73.10	4849.0
74.00	18312.0
75.10	55632.0
76.10	4560.0
77.00	539.0
78.10	538.0
78.90	3304.0
80.00	829.0
81.00	3559.0
81.90	639.0
82.90	163.0
86.00	139.0
87.00	4710.0
88.00	5022.0
90.90	480.0
92.00	2999.0
93.00	4992.0
94.00	13093.0
95.00	115424.0
96.00	7384.0
97.00	280.0
104.00	466.0
104.80	179.0
105.90	529.0
106.80	101.0
110.90	125.0
114.90	170.0
115.90	410.0
116.90	784.0
117.90	405.0
119.00	656.0
127.90	440.0
128.90	237.0
129.80	437.0
130.90	224.0
134.90	211.0
136.80	218.0
140.90	1384.0
141.90	186.0
142.90	1605.0
143.90	115.0
144.90	396.0
145.80	233.0
147.90	245.0
149.80	150.0
152.80	120.0
154.90	275.0
156.90	232.0
159.00	145.0
160.90	158.0
170.80	212.0
172.00	1467.0
173.00	1099.0
174.00	102728.0
175.00	7768.0
176.00	98984.0
177.00	6245.0
178.00	175.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226

m/z	Abundance
36.00	659.0
37.00	3084.0
38.00	3259.0
39.00	1443.0
39.90	278.0
42.90	119.0
43.90	714.0
45.00	704.0
46.10	141.0
47.00	1106.0
48.00	660.0
49.10	3153.0
50.10	15496.0
51.00	4856.0
52.00	232.0
53.10	181.0
54.00	109.0
54.90	296.0
55.90	1182.0
57.00	2458.0
58.00	136.0
60.00	789.0
61.00	4425.0
62.10	4759.0
63.00	3617.0
63.90	532.0
65.00	980.0
67.10	275.0
68.00	9251.0
69.00	9610.0
70.00	712.0
72.10	496.0
73.10	4305.0
74.00	16616.0
75.10	49824.0
76.00	4040.0
77.00	562.0
78.10	396.0
78.90	3113.0
80.00	778.0
81.00	3237.0
82.00	589.0
82.90	171.0
86.00	115.0
86.90	4231.0
88.00	4416.0
90.90	445.0
92.00	2672.0
93.00	4690.0
94.00	11928.0
95.00	104872.0
96.00	6453.0
97.00	249.0
104.00	432.0
104.80	138.0
105.90	493.0
110.90	137.0
114.90	161.0
115.90	397.0
116.90	791.0
117.90	410.0
119.00	613.0
127.80	369.0
128.90	206.0
129.80	423.0
130.90	186.0
134.90	214.0
136.80	206.0
140.90	1226.0
141.90	165.0
142.90	1429.0
143.90	109.0
145.00	321.0
145.90	208.0
147.90	231.0
149.90	105.0
152.80	125.0
154.90	263.0
156.90	218.0
158.90	148.0
160.90	125.0
170.90	222.0
171.90	1415.0
173.00	1008.0
174.00	95864.0
175.00	7056.0
176.00	92664.0
177.00	5706.0
177.90	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226