
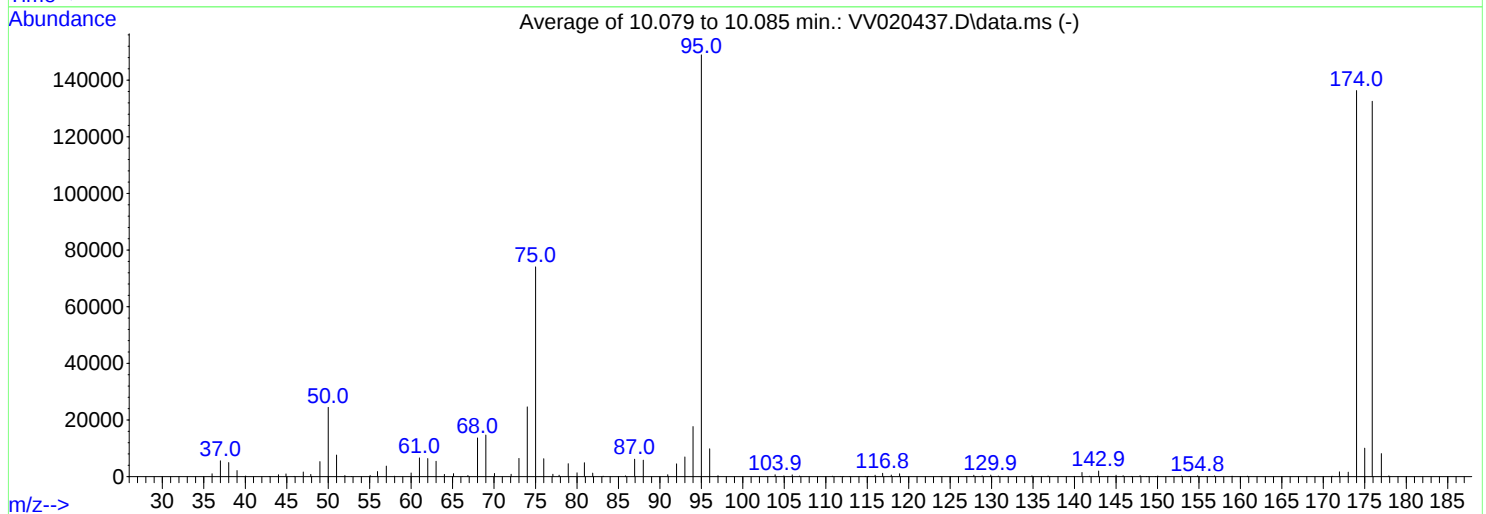


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030321\
 Data File : VV020437.D
 Acq On : 03 Mar 2021 09:00
 Operator : SY/MD
 Sample : BFB35
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB308

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030221.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Mar 04 00:23:40 2021

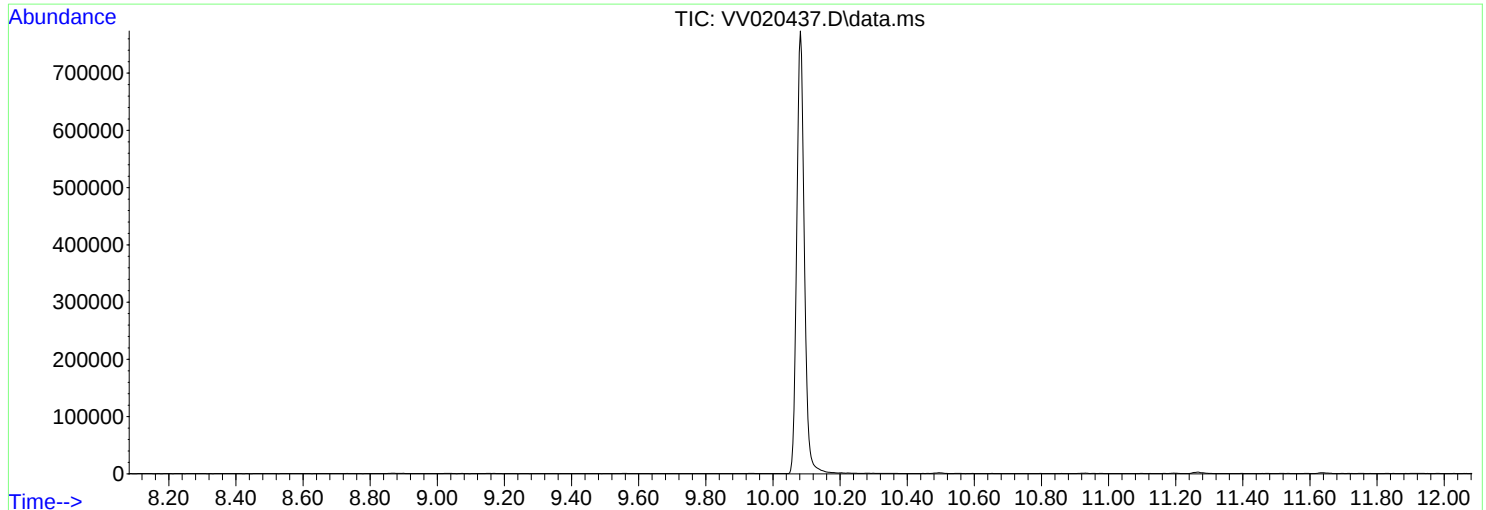

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	24443	PASS
75	95	30	80	49.7	74064	PASS
95	95	100	100	100.0	148949	PASS
96	95	5	9	6.6	9831	PASS
173	174	0.00	2	1.2	1598	PASS
174	95	50	120	91.5	136355	PASS
175	174	5	9	7.4	10038	PASS
176	174	95	101	97.2	132552	PASS
177	176	5	9	6.2	8162	PASS

m/z	Abundance
36.00	1021.0
37.00	5752.0
38.00	4833.0
39.00	2211.0
40.00	223.0
44.00	1046.0
44.90	984.0
45.90	174.0
47.00	1663.0
47.90	876.0
49.00	5394.0
50.00	24600.0
51.00	7749.0
52.00	408.0
52.80	116.0
55.10	430.0
56.00	1773.0
57.00	3804.0
58.00	201.0
60.00	1382.0
61.00	6482.0
62.00	6551.0
63.00	5334.0
64.00	838.0
65.10	1047.0
66.10	149.0
66.90	419.0
68.00	13354.0
69.00	14590.0
70.10	1143.0
72.00	849.0
73.00	6354.0
74.00	24160.0
75.00	73608.0
76.00	6501.0
77.10	732.0
77.90	470.0
79.00	4606.0
80.00	1424.0
80.90	4827.0
81.90	1222.0
83.10	189.0
85.90	347.0
87.00	6201.0
88.00	5886.0
91.00	616.0
92.00	4392.0
93.00	6696.0
94.00	17992.0
95.00	149312.0
96.00	9791.0
97.00	385.0
102.90	113.0
103.90	662.0
104.90	259.0
105.90	668.0
106.90	214.0
110.80	185.0
112.90	108.0
114.80	154.0
116.00	510.0
116.80	1144.0
117.90	553.0
118.90	987.0
127.90	444.0
128.90	330.0
129.90	623.0
130.80	244.0
134.80	298.0
136.80	270.0
139.90	133.0
140.90	1470.0
141.80	191.0
142.90	1827.0
144.10	125.0
144.90	530.0
145.80	298.0
146.90	114.0
147.80	325.0
148.70	128.0
149.80	199.0
150.10	187.0
152.90	187.0
153.80	118.0
154.90	370.0
156.90	279.0
159.00	135.0
161.00	165.0
171.10	237.0
172.00	1731.0
173.00	1545.0
174.00	130984.0

Instrument :
MSVOA_V
ClientSampleId :
BFB308

175.00	9877.0
175.90	127832.0
177.00	8279.0
177.90	286.0

Instrument :
MSVOA_V
ClientSampleId :
BFB308

m/z	Abundance
36.00	1077.0
37.00	5830.0
38.00	5118.0
39.00	2180.0
40.10	253.0
44.00	1123.0
44.90	971.0
45.90	131.0
47.00	1741.0
47.90	815.0
49.00	5548.0
50.00	25256.0
51.00	7941.0
52.00	400.0
55.10	450.0
56.00	1839.0
57.00	3884.0
58.00	206.0
60.00	1388.0
61.00	6853.0
62.00	6623.0
63.00	5631.0
64.00	841.0
65.10	1135.0
66.20	113.0
66.90	438.0
68.00	14157.0
69.00	15222.0
70.00	1176.0
72.10	915.0
73.00	6692.0
74.00	25648.0
75.00	76680.0
76.00	6604.0
77.10	892.0
77.90	506.0
78.90	4677.0
80.00	1422.0
80.90	5118.0
81.90	1276.0
83.10	151.0
85.90	292.0
86.90	6332.0
88.00	6042.0
91.00	709.0
92.00	4665.0
93.00	7230.0
94.00	18360.0
95.00	154112.0
96.00	10173.0
97.00	349.0
102.90	108.0
103.90	676.0
104.90	272.0
105.90	649.0
106.80	204.0
110.80	177.0
112.20	114.0
112.90	103.0
114.70	130.0
115.20	143.0
115.90	516.0
116.80	1206.0
117.90	602.0
118.90	1081.0
123.80	102.0
127.90	510.0
128.80	310.0
129.90	584.0
130.80	295.0
134.80	290.0
136.80	246.0
139.90	142.0
140.90	1532.0
141.80	186.0
142.90	2055.0
144.00	145.0
145.00	502.0
145.90	334.0
146.80	147.0
147.90	353.0
148.90	135.0
150.10	221.0
152.90	242.0
153.80	138.0
154.80	365.0
155.90	104.0
156.90	313.0
159.00	159.0
160.80	189.0
171.00	188.0
172.00	1708.0

Instrument :
MSVOA_V
ClientSampleId :
BFB308

173.00	1640.0
174.00	141056.0
175.00	10372.0
175.90	137024.0
177.00	8444.0
177.90	313.0

Instrument :
MSVOA_V
ClientSampleId :
BFB308

m/z	Abundance
36.00	1016.0
37.00	5238.0
38.00	4922.0
39.00	2004.0
40.10	262.0
42.90	103.0
44.00	1155.0
44.90	892.0
47.00	1605.0
47.90	713.0
49.00	4984.0
50.00	23472.0
51.00	7207.0
52.00	360.0
55.00	413.0
55.90	1771.0
57.00	3566.0
58.00	177.0
60.00	1194.0
61.00	6492.0
62.00	6002.0
63.00	5400.0
64.00	717.0
65.10	1062.0
66.80	350.0
68.00	13441.0
69.00	14284.0
70.00	1071.0
72.10	846.0
73.00	6315.0
74.00	24192.0
75.00	71904.0
76.00	5903.0
77.10	949.0
77.80	550.0
78.90	4491.0
80.00	1225.0
80.90	4841.0
81.90	1180.0
83.20	115.0
85.80	236.0
86.90	5909.0
88.00	5601.0
90.90	717.0
92.00	4561.0
93.00	6962.0
94.00	16672.0
95.00	143424.0
96.00	9530.0
97.00	306.0
103.90	636.0
105.00	269.0
106.00	599.0
106.80	189.0
110.80	146.0
111.80	102.0
112.10	114.0
115.10	142.0
115.90	518.0
116.90	1156.0
117.90	546.0
118.90	1072.0
126.90	105.0
127.80	537.0
128.80	258.0
129.90	535.0
130.80	246.0
134.90	281.0
136.80	232.0
140.00	130.0
140.90	1450.0
141.80	139.0
142.90	2051.0
144.00	134.0
145.10	451.0
145.90	332.0
146.90	130.0
148.00	321.0
148.90	116.0
150.00	219.0
152.90	228.0
153.80	140.0
154.80	381.0
156.90	322.0
159.00	150.0
160.80	186.0
171.10	127.0
171.90	1620.0
173.00	1609.0
174.00	137024.0
175.00	9866.0
175.90	132800.0

Instrument :
MSVOA_V
ClientSampleId :
BFB308

177.00	7764.0
177.90	268.0

Instrument :
MSVOA_V
ClientSampleId :
BFB308

m/z	Abundance
39.80	161.0
44.00	425.0

Instrument :
MSVOA_V
ClientSampleId :
BFB308