




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
 Data File : VV030136.D
 Acq On : 03 Mar 2023 13:36
 Operator : SY/MD
 Sample : 01769-02DL 500X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBYL2DL

Manual IntegrationsAPPROVED

Quant Time: Mar 03 22:28:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 03 22:25:34 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/06/2023
 Supervised By :Mahesh Dadoda 03/06/2023

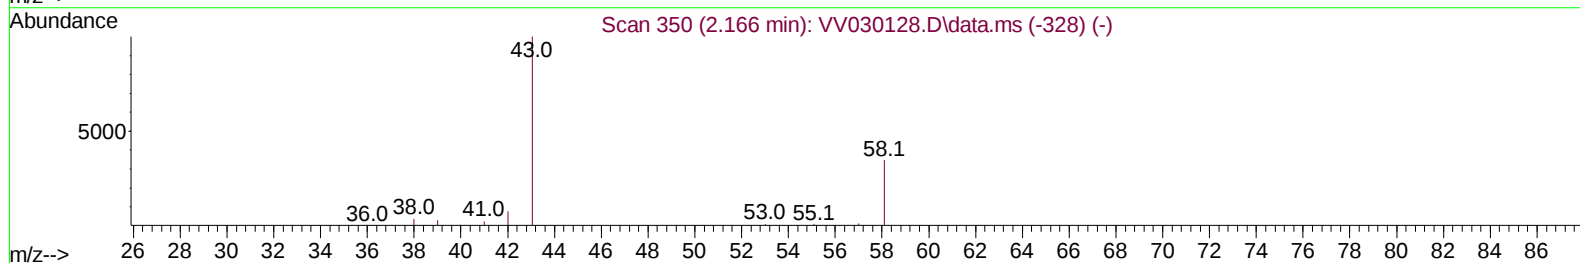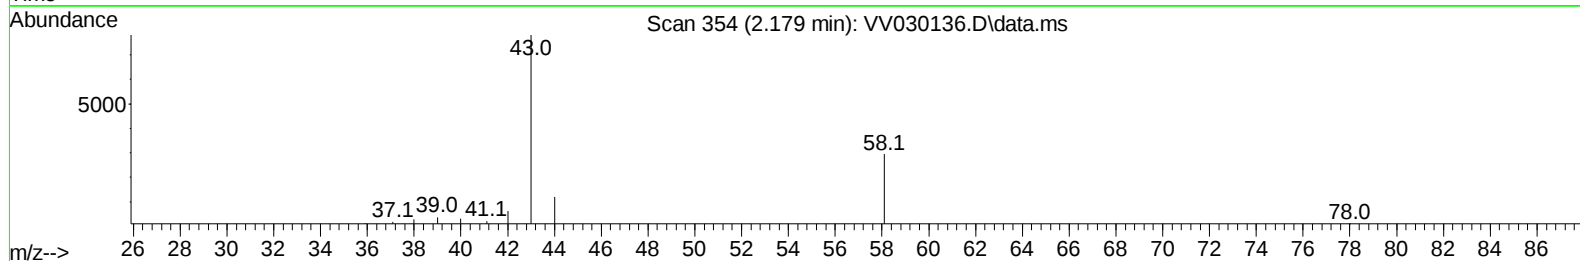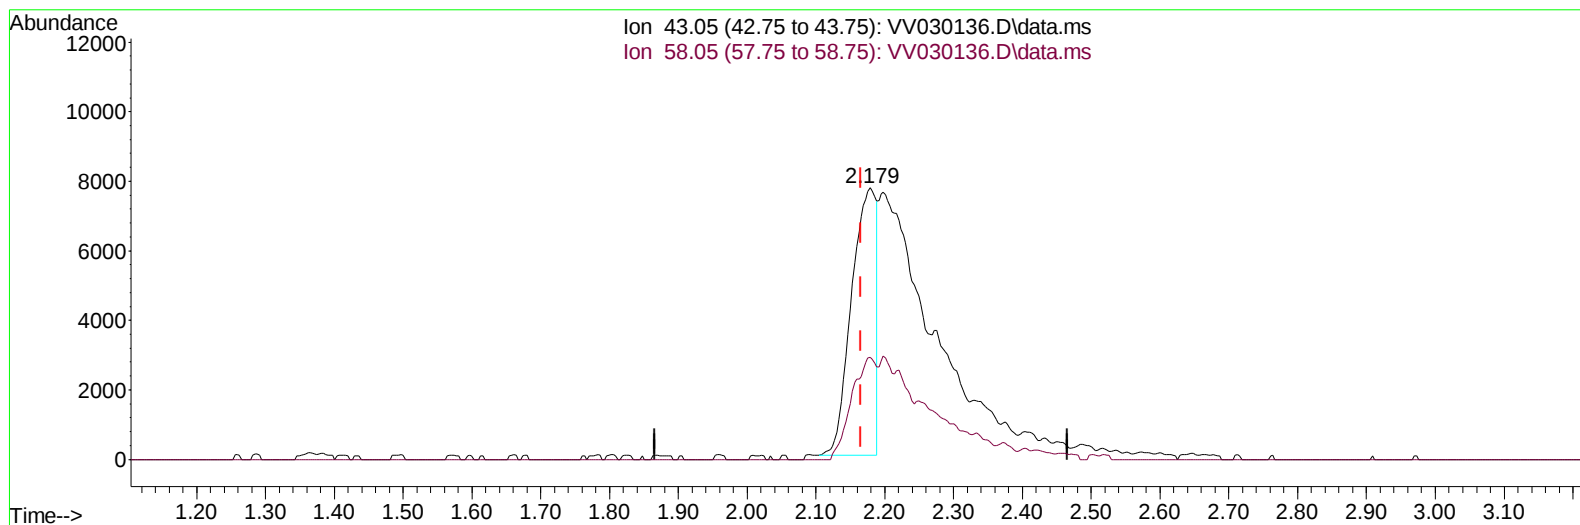

TIC: VV030136.D\data.ms

(13) Acetone (T)

2.179min (+ 0.013) 15.85 ug/L

response 19119

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	14.70	40.45#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
 Data File : VV030136.D
 Acq On : 03 Mar 2023 13:36
 Operator : SY/MD
 Sample : 01769-02DL 500X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBYL2DL

Manual IntegrationsAPPROVED

Quant Time: Mar 03 22:28:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 03 22:25:34 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/06/2023
 Supervised By :Mahesh Dadoda 03/06/2023

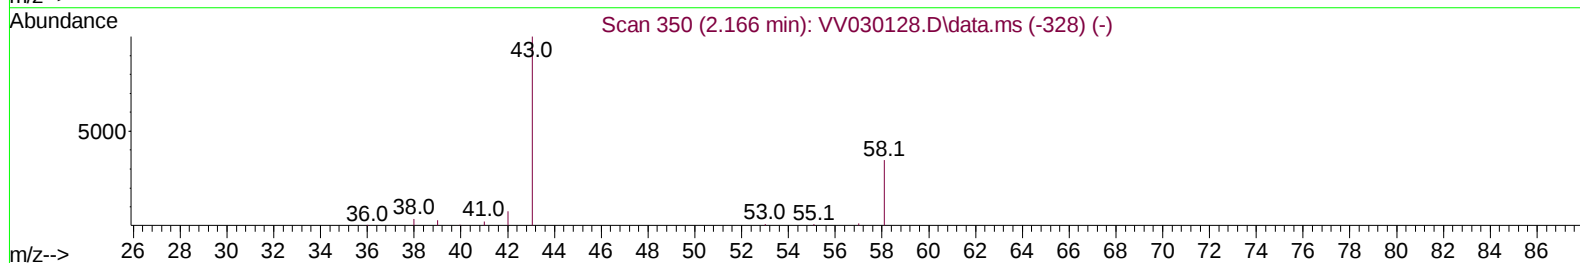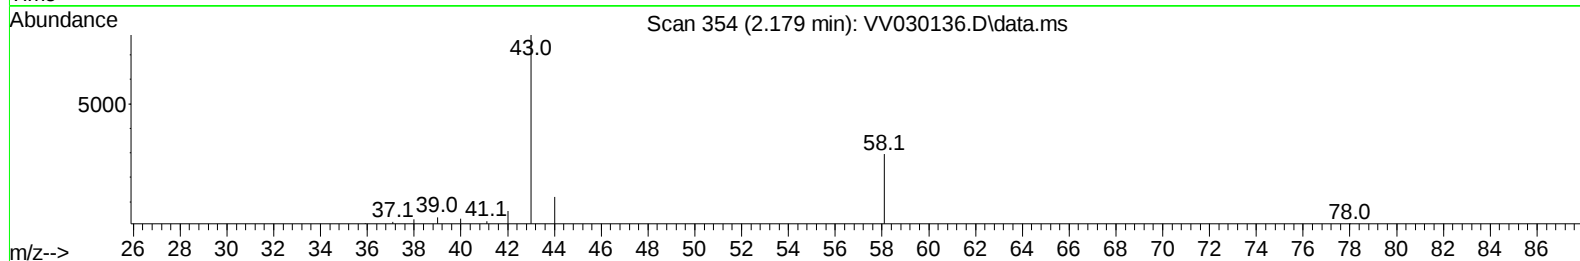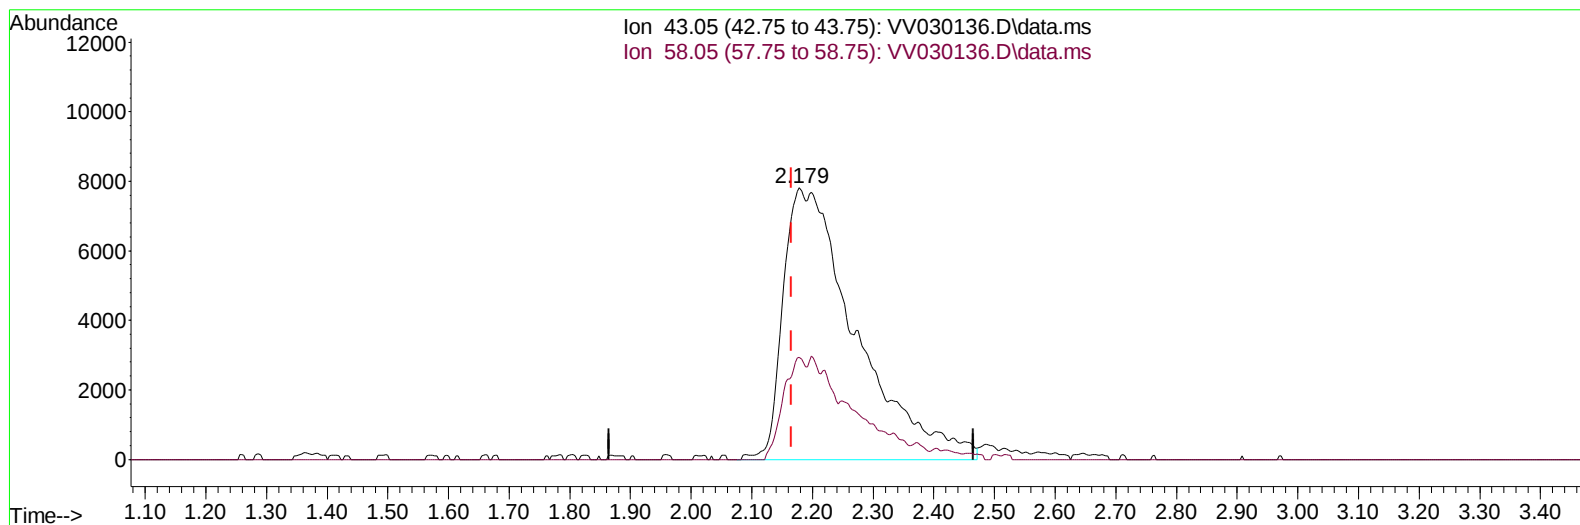

TIC: VV030136.D\data.ms

(13) Acetone (T)

2.179min (+ 0.013) 53.83 ug/L m

response 64955

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	14.70	11.91
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
 Data File : VV030136.D
 Acq On : 03 Mar 2023 13:36
 Operator : SY/MD
 Sample : 01769-02DL 500X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBYL2DL

Manual IntegrationsAPPROVED

Quant Time: Mar 03 22:28:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 03 22:25:34 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/06/2023
 Supervised By :Mahesh Dadoda 03/06/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.545	114		136843	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117		135307	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152		65083	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.282	65		34979	3.950	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130			Recovery =	79.000%		
7) Chloroethane-d5	1.536	69		39710	4.778	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130			Recovery =	95.600%		
11) 1,1-Dichloroethene-d2	2.066	63		60731	3.336	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125			Recovery =	66.800%		
20) 2-Butanone-d5	3.854	46		79392	48.632	ug/L	0.02
Spiked Amount 50.000	Range 40 - 130			Recovery =	97.260%		
24) Chloroform-d	4.265	84		90582	5.008	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125			Recovery =	100.200%		
26) 1,2-Dichloroethane-d4	4.960	65		38631	5.232	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130			Recovery =	104.600%		
32) Benzene-d6	4.973	84		158177	4.345	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125			Recovery =	86.800%		
36) 1,2-Dichloropropane-d6	6.002	67		52843	4.824	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140			Recovery =	96.400%		
41) Toluene-d8	7.252	98		129852	3.763	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130			Recovery =	75.200%		
43) trans-1,3-Dichloroprop...	7.564	79		15437	4.119	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130			Recovery =	82.400%		
46) 2-Hexanone-d5	8.040	63		75167	48.484	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130			Recovery =	96.960%		
56) 1,1,2,2-Tetrachloroeth...	10.162	84		41342	5.305	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120			Recovery =	106.200%		
66) 1,2-Dichlorobenzene-d4	11.570	152		52965	4.810	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120			Recovery =	96.200%		
Target Compounds							
13) Acetone	2.179	43		64955m	53.834	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
Data File : VV030136.D
Acq On : 03 Mar 2023 13:36
Operator : SY/MD
Sample : 01769-02DL 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
DBYL2DL

Manual IntegrationsAPPROVED

Quant Time: Mar 03 22:28:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 03 22:25:34 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 03/06/2023
Supervised By :Mahesh Dadoda 03/06/2023

