

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
 Data File : VV030129.D
 Acq On : 03 Mar 2023 10:08
 Operator : SY/MD
 Sample : VV0303WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK307

Quant Time: Mar 03 22:26:18 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 03 22:25:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	134453	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	134770	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	66064	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	37771	4.342	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.800%
7) Chloroethane-d5	1.536	69	40726	4.987	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.800%
11) 1,1-Dichloroethene-d2	2.063	63	62288	3.483	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.600%
20) 2-Butanone-d5	3.844	46	78057	48.665	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.320%
24) Chloroform-d	4.259	84	91665	5.158	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.200%
26) 1,2-Dichloroethane-d4	4.957	65	40157	5.535	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.800%
32) Benzene-d6	4.970	84	160219	4.418	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.400%
36) 1,2-Dichloropropane-d6	5.998	67	54324	4.979	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.600%
41) Toluene-d8	7.252	98	130412	3.794	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.800%
43) trans-1,3-Dichloroprop...	7.564	79	16359	4.383	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.600%
46) 2-Hexanone-d5	8.037	63	74586	48.301	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.600%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	42362	5.458	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	109.200%
66) 1,2-Dichlorobenzene-d4	11.571	152	54497	4.876	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.600%
Target Compounds						
16) Methylene chloride	2.455	84	3813	0.346	ug/L	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
Data File : VV030129.D
Acq On : 03 Mar 2023 10:08
Operator : SY/MD
Sample : VV0303WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK307


Quant Time: Mar 03 22:26:18 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 03 22:25:34 2023
Response via : Initial Calibration

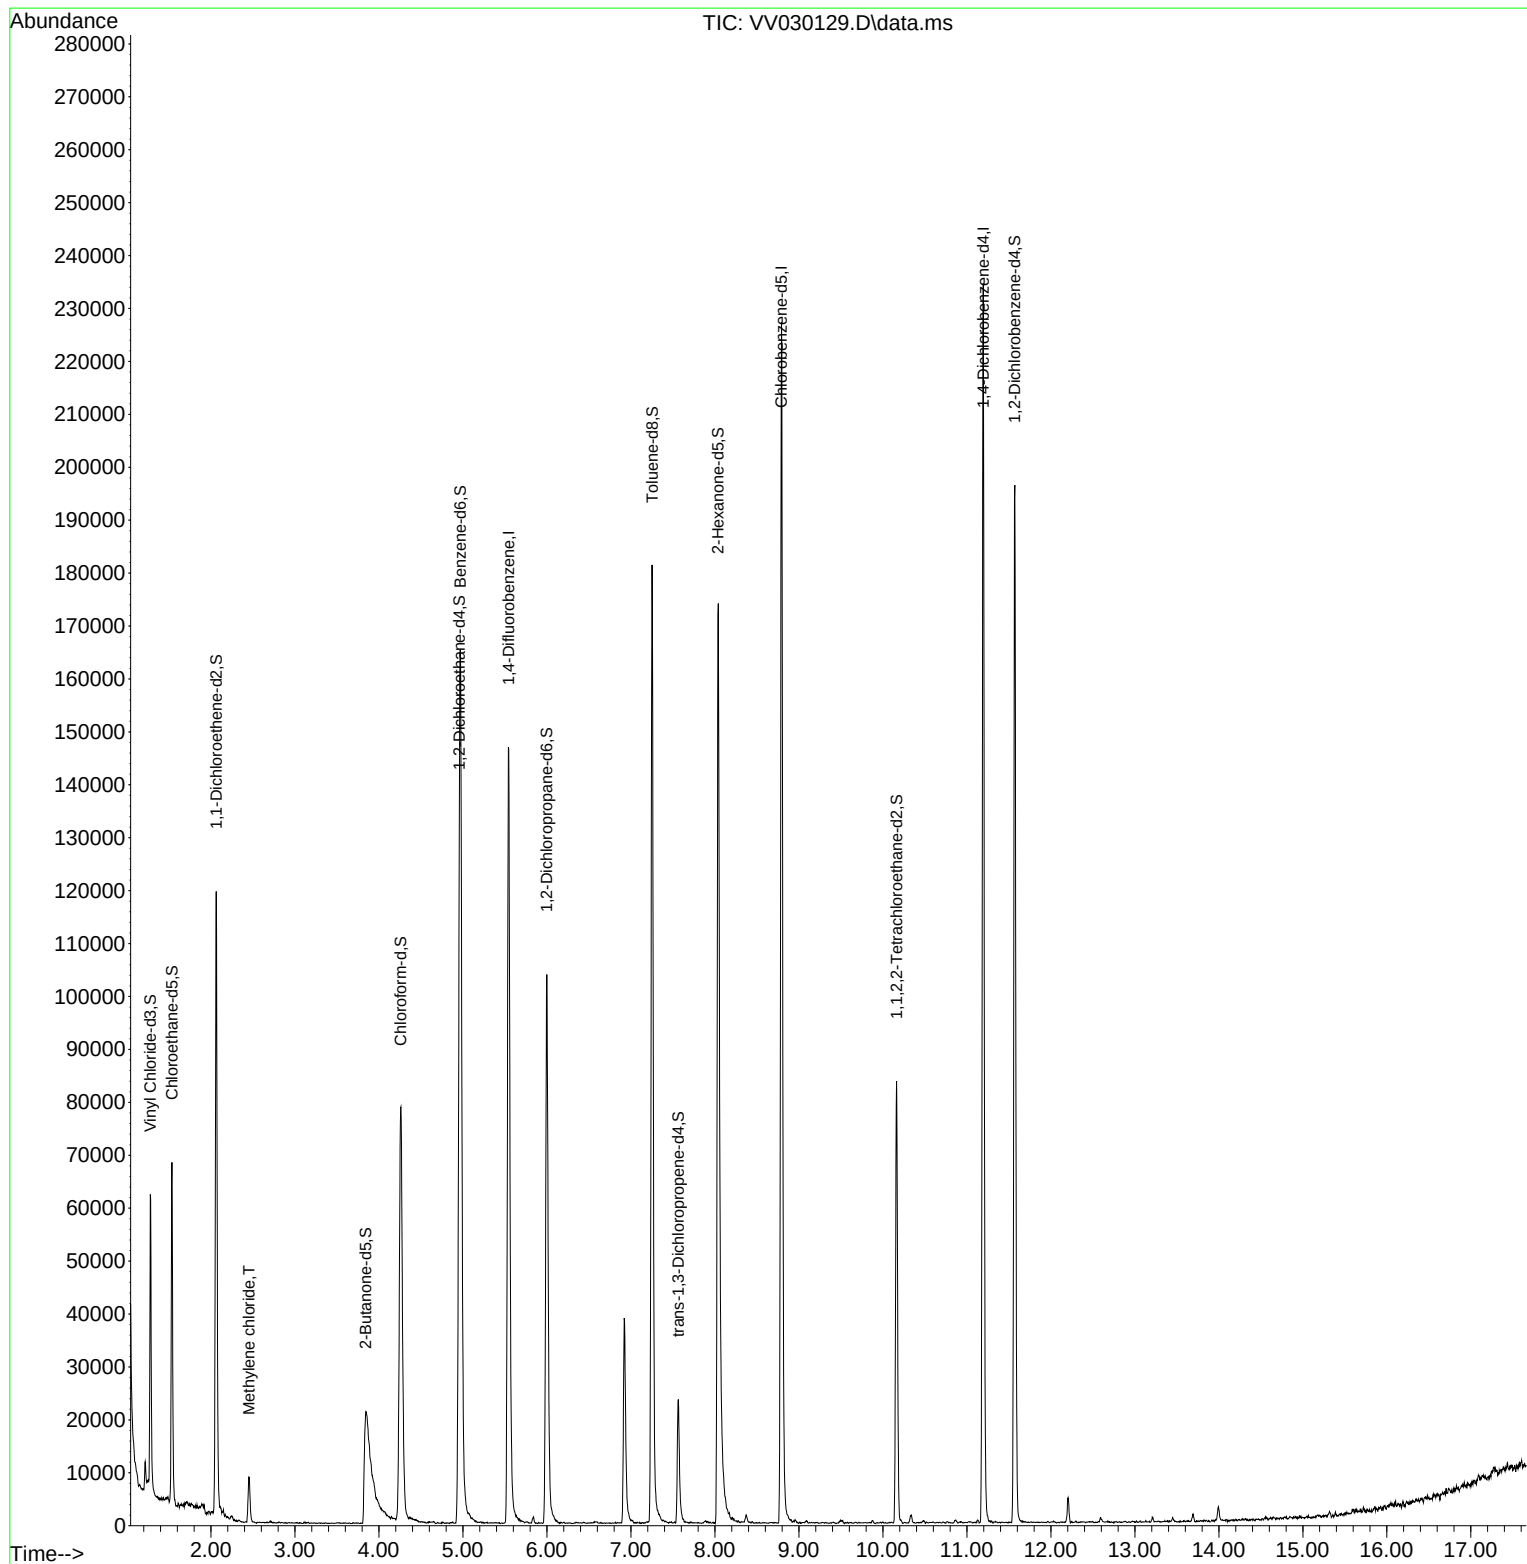

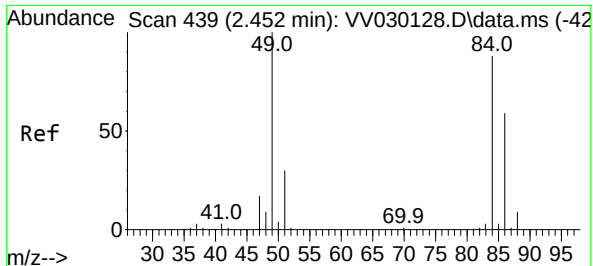

#16
Methylene chloride
Concen: 0.346 ug/L
RT: 2.455 min Scan# 44
Delta R.T. 0.003 min
Lab File: VV030129.D
Acq: 03 Mar 2023 10:08

Instrument :
MSVOA_V
ClientSampleId :
VBLK307

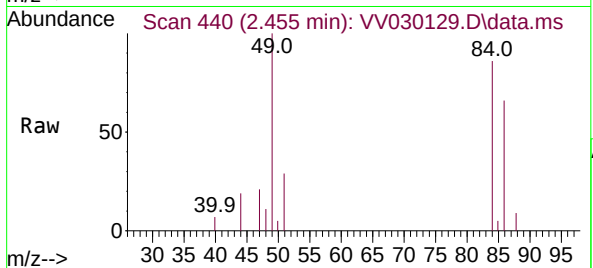

Tgt Ion: 84 Resp: 3813
Ion Ratio Lower Upper
84 100
86 76.7 44.7 83.1
49 116.2 78.8 146.3

