

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
 Data File : VV030134.D
 Acq On : 03 Mar 2023 12:51
 Operator : SY/MD
 Sample : 01769-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBYL6

Quant Time: Mar 03 22:27:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 03 22:25:34 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	140347	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	136678	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	68147	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	37562	4.136	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	82.800%	
7) Chloroethane-d5	1.536	69	40996	4.809	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	96.200%	
11) 1,1-Dichloroethene-d2	2.063	63	61879	3.314	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	66.200%	
20) 2-Butanone-d5	3.828	46	87354	52.174	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	104.340%	
24) Chloroform-d	4.259	84	92910	5.009	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	100.200%	
26) 1,2-Dichloroethane-d4	4.954	65	39879	5.266	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	105.400%	
32) Benzene-d6	4.970	84	166399	4.525	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.400%	
36) 1,2-Dichloropropane-d6	5.998	67	53507	4.836	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	96.800%	
41) Toluene-d8	7.252	98	137506	3.944	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	78.800%	
43) trans-1,3-Dichloroprop...	7.561	79	16330	4.314	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	86.200%	
46) 2-Hexanone-d5	8.037	63	77604	49.554	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	99.100%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84	42195	5.361	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	107.200%	
66) 1,2-Dichlorobenzene-d4	11.571	152	55643	4.826	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	96.600%	
Target Compounds						
13) Acetone	2.166	43	46126	37.274	ug/L	# 43
42) Toluene	7.326	91	7892	0.195	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
Data File : VV030134.D
Acq On : 03 Mar 2023 12:51
Operator : SY/MD
Sample : 01769-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBYL6

Quant Time: Mar 03 22:27:38 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 03 22:25:34 2023
Response via : Initial Calibration

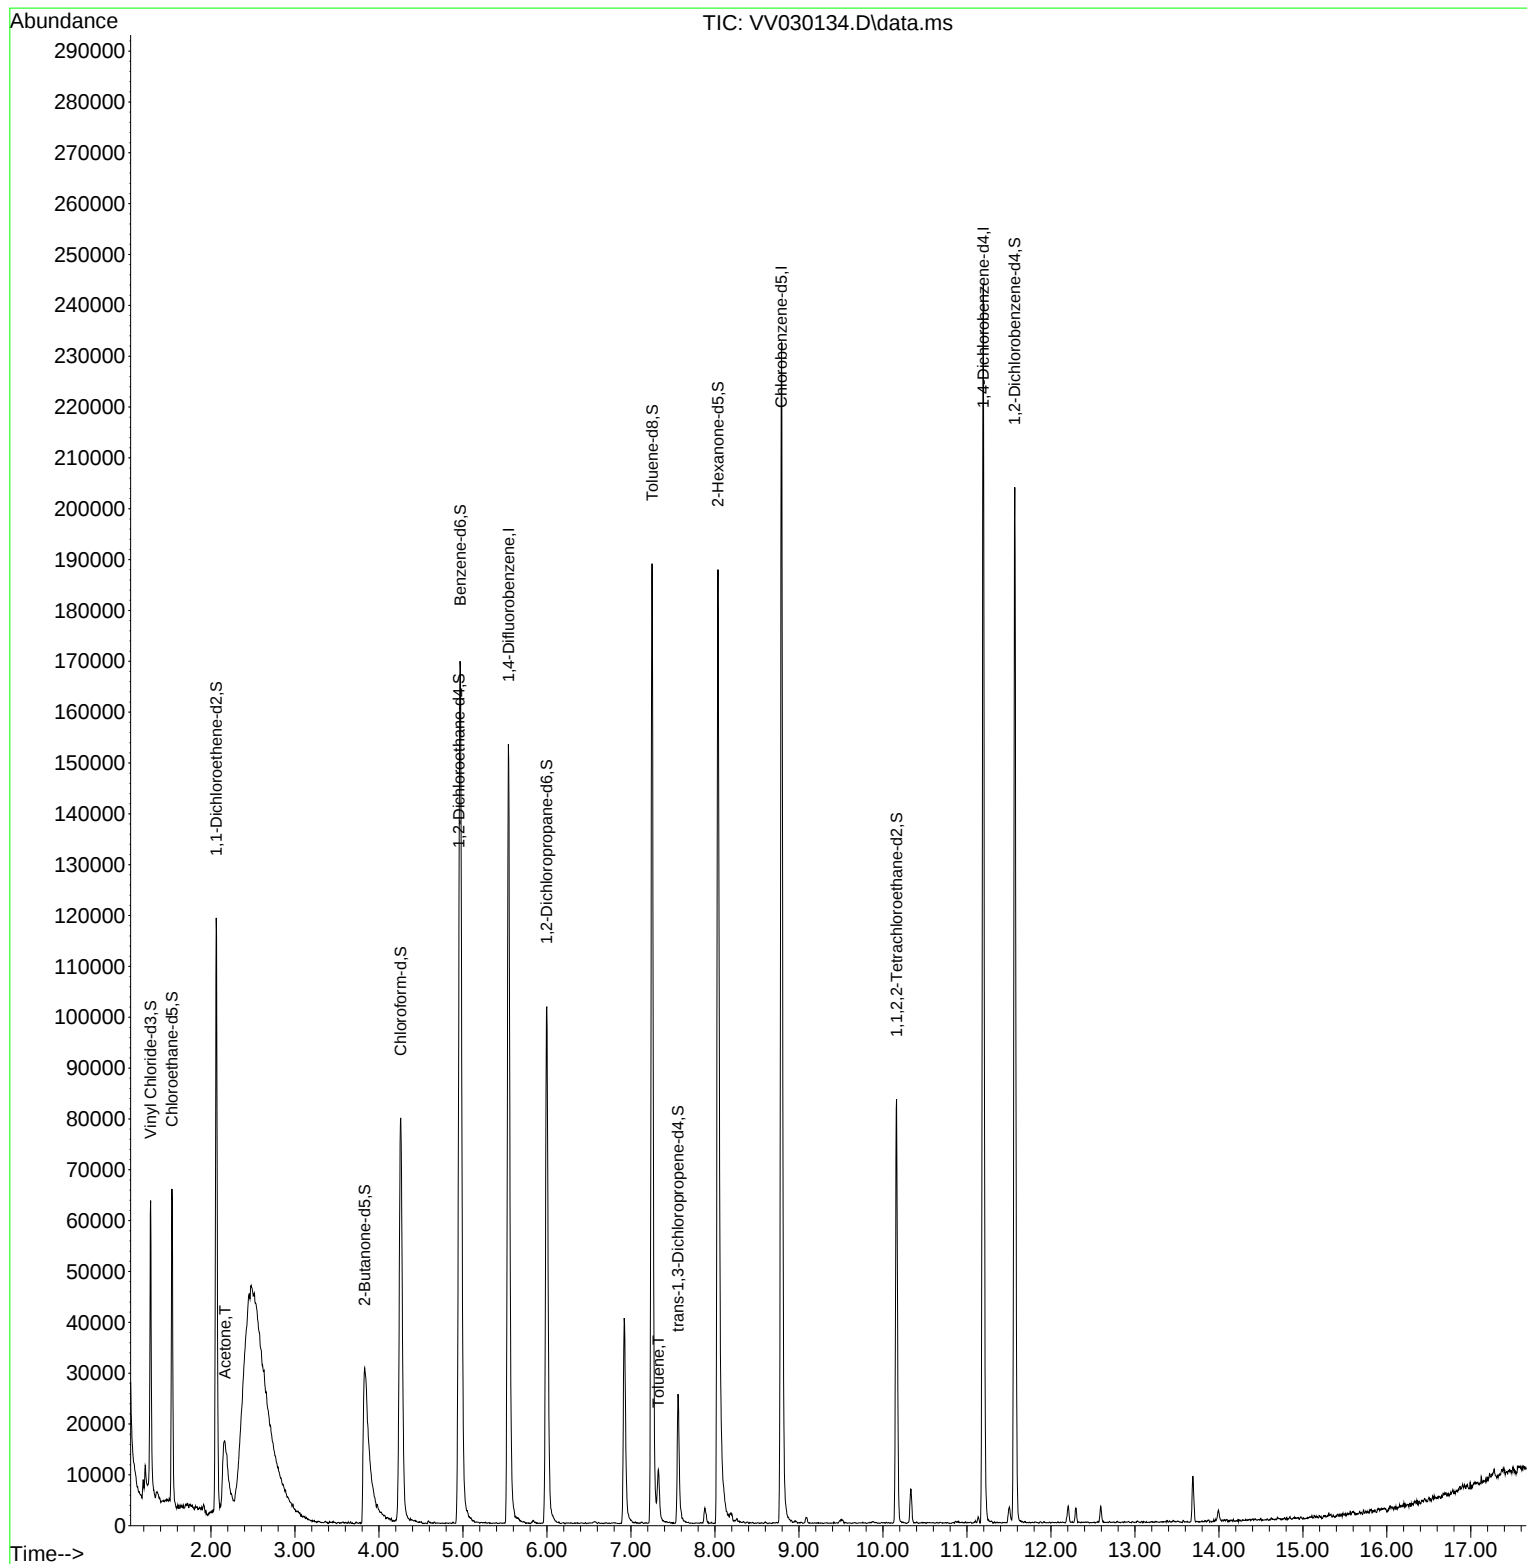

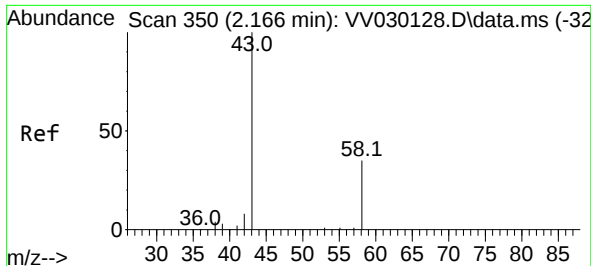

#13

Acetone

Concen: 37.274 ug/L

RT: 2.166 min Scan# 350

Delta R.T. 0.000 min

Lab File: VV030134.D

Acq: 03 Mar 2023 12:51

Instrument :

MSVOA_V

ClientSampleId :





DBYL6

Tgt Ion: 43 Resp: 46126

Ion Ratio Lower Upper

43 100

58 38.4 0.0 29.4#

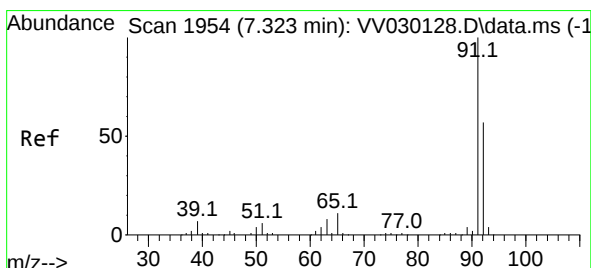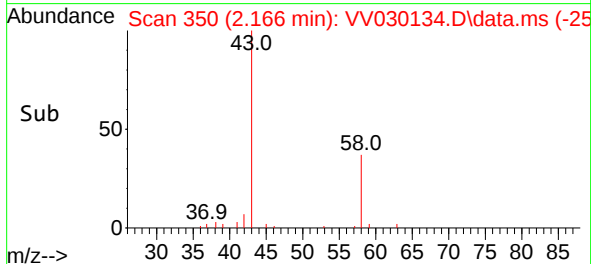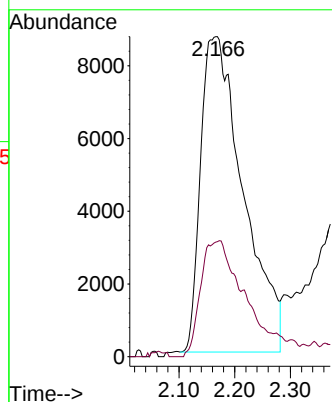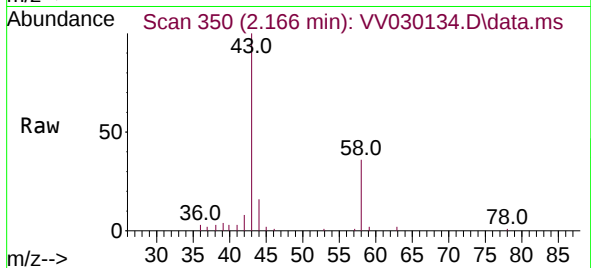

#42

Toluene

Concen: 0.195 ug/L

RT: 7.326 min Scan# 1955

Delta R.T. 0.003 min

Lab File: VV030134.D

Acq: 03 Mar 2023 12:51

Tgt Ion: 91 Resp: 7892

Ion Ratio Lower Upper

91 100

92 48.7 39.6 73.6

