

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
 Data File : VV030136.D
 Acq On : 03 Mar 2023 13:36
 Operator : SY/MD
 Sample : 01769-02DL 500X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBYL2DL

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 03/06/2023
 Supervised By :Mahesh Dadoda 03/06/2023

Quant Time: Mar 03 22:28:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 03 22:25:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	136843	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	135307	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	65083	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	34979	3.950	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	79.000%	
7) Chloroethane-d5	1.536	69	39710	4.778	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	95.600%	
11) 1,1-Dichloroethene-d2	2.066	63	60731	3.336	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	66.800%	
20) 2-Butanone-d5	3.854	46	79392	48.632	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	97.260%	
24) Chloroform-d	4.265	84	90582	5.008	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	100.200%	
26) 1,2-Dichloroethane-d4	4.960	65	38631	5.232	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	104.600%	
32) Benzene-d6	4.973	84	158177	4.345	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	86.800%	
36) 1,2-Dichloropropane-d6	6.002	67	52843	4.824	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	96.400%	
41) Toluene-d8	7.252	98	129852	3.763	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	75.200%	
43) trans-1,3-Dichloroprop...	7.564	79	15437	4.119	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	82.400%	
46) 2-Hexanone-d5	8.040	63	75167	48.484	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	96.960%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84	41342	5.305	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	106.200%	
66) 1,2-Dichlorobenzene-d4	11.570	152	52965	4.810	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	96.200%	
Target Compounds					Qvalue	
13) Acetone	2.179	43	64955m	53.834	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
Data File : VV030136.D
Acq On : 03 Mar 2023 13:36
Operator : SY/MD
Sample : 01769-02DL 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
DBYL2DL

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 03/06/2023
Supervised By :Mahesh Dadoda 03/06/2023


Quant Time: Mar 03 22:28:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 03 22:25:34 2023
Response via : Initial Calibration

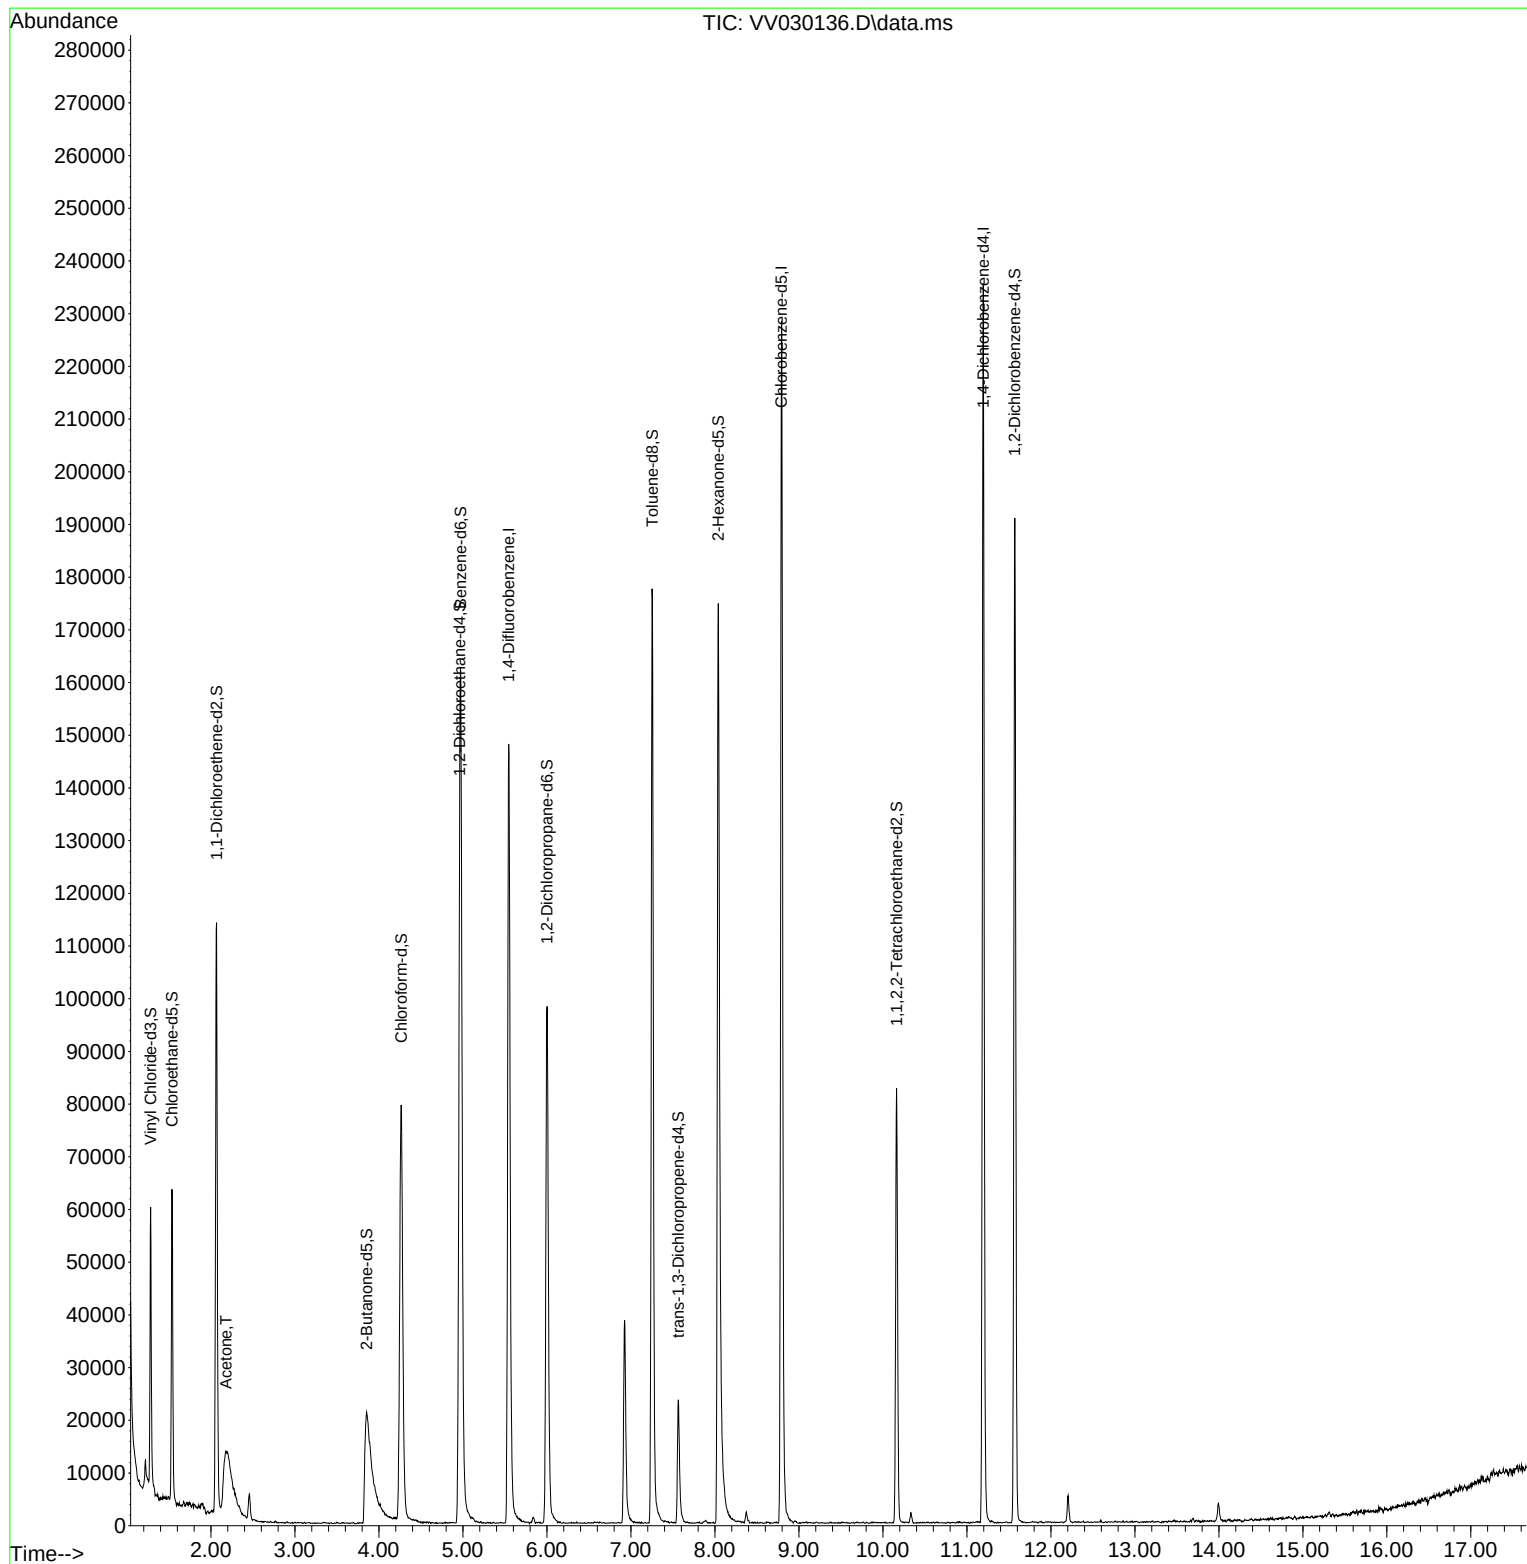

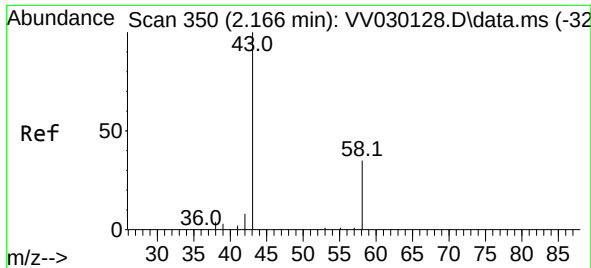

#13
 Acetone
 Concen: 53.834 ug/L m
 RT: 2.179 min Scan# 30
 Delta R.T. 0.013 min
 Lab File: VV030136.D
 Acq: 03 Mar 2023 13:36

Instrument :
 MSVOA_V
 ClientSampleId :
 DBYL2DL

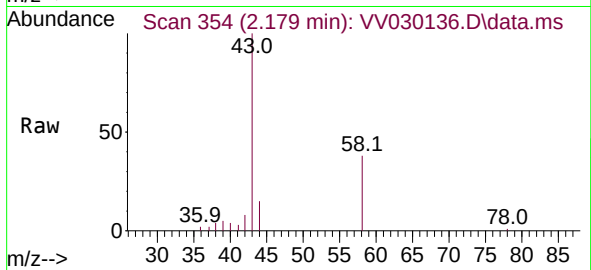

Tgt Ion: 43 Resp: 6495
 Ion Ratio Lower Upper
 43 100
 58 11.9 0.0 29.4

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 03/06/2023
 Supervised By :Mahesh Dadoda 03/06/2023

