

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
 Data File : VV030129.D
 Acq On : 03 Mar 2023 10:08
 Operator : SY/MD
 Sample : VV0303WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK307

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030129.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	60	rBV2	5307	5844	1.38%	0.163%
2	1.278	68	74	96	rVB	57133	65930	15.59%	1.833%
3	1.536	146	154	169	rVB	64942	75774	17.92%	2.107%
4	2.063	307	318	331	rBV	117409	170977	40.43%	4.755%
5	2.452	431	439	452	rBV2	8557	14010	3.31%	0.390%
6	3.844	859	872	910	rBV	21139	114786	27.15%	3.192%
7	4.262	983	1002	1030	rBV	78030	202805	47.96%	5.640%
8	4.970	1205	1222	1250	rBV2	164975	422850	100.00%	11.759%
9	5.542	1383	1400	1437	rBV	146621	305522	72.25%	8.496%
10	5.998	1526	1542	1575	rBV	103714	215022	50.85%	5.980%
11	6.921	1818	1829	1852	rBV	38719	73197	17.31%	2.036%
12	7.252	1919	1932	1952	rBV	180861	323243	76.44%	8.989%
13	7.564	2019	2029	2046	rBV	23348	43185	10.21%	1.201%
14	8.040	2166	2177	2216	rBV	173746	368255	87.09%	10.241%
15	8.793	2400	2411	2445	rBV	226885	380880	90.07%	10.592%
16	10.162	2826	2837	2851	rBV	83510	133261	31.51%	3.706%
17	11.194	3146	3158	3174	rBV	234125	363868	86.05%	10.119%
18	11.571	3263	3275	3302	rBV	196052	309464	73.19%	8.606%
19	12.204	3463	3472	3481	rVB3	4761	7059	1.67%	0.196%




Sum of corrected areas: 3595932

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
Data File : VV030129.D
Acq On : 03 Mar 2023 10:08
Operator : SY/MD
Sample : VV0303WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK307

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

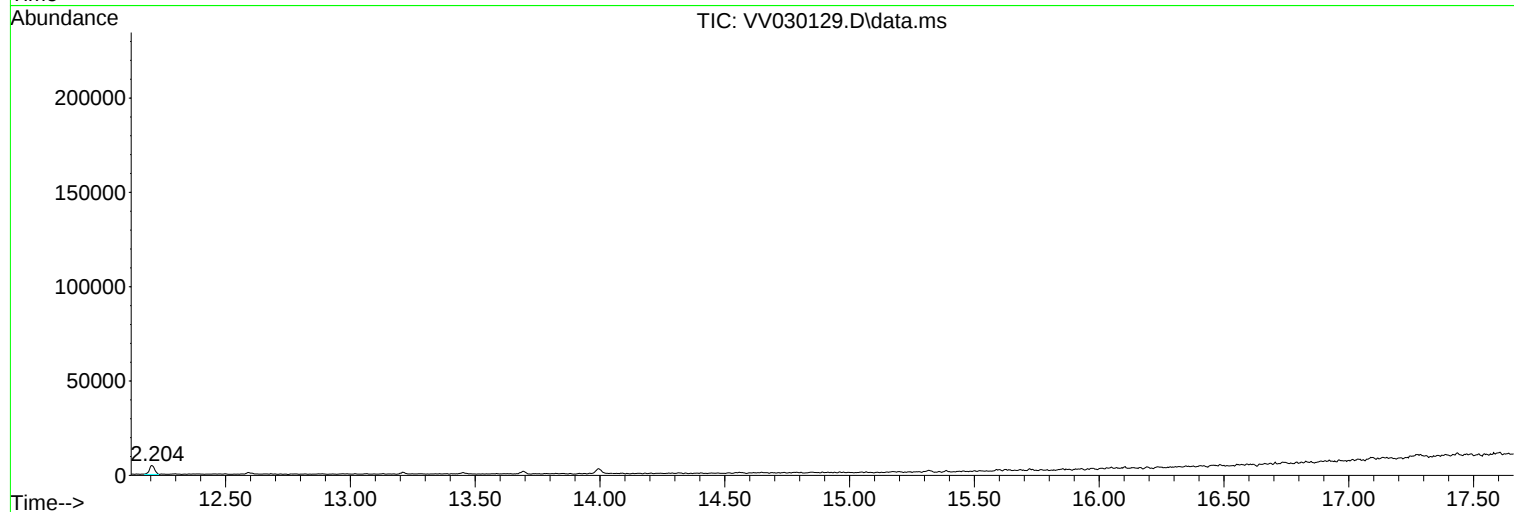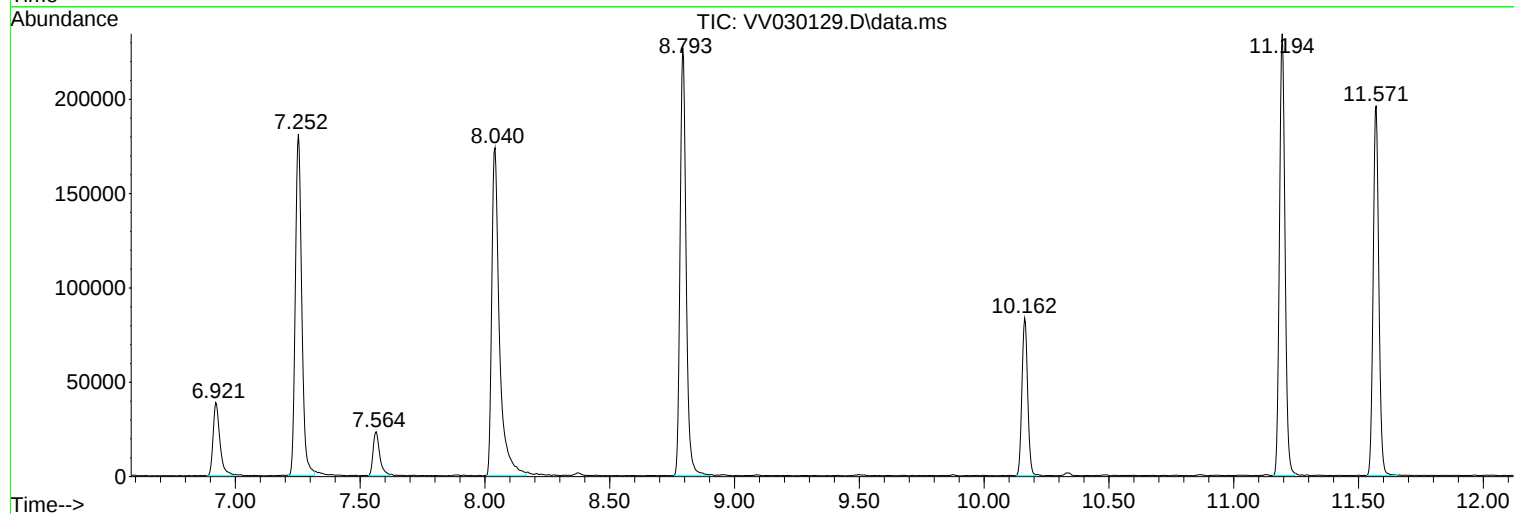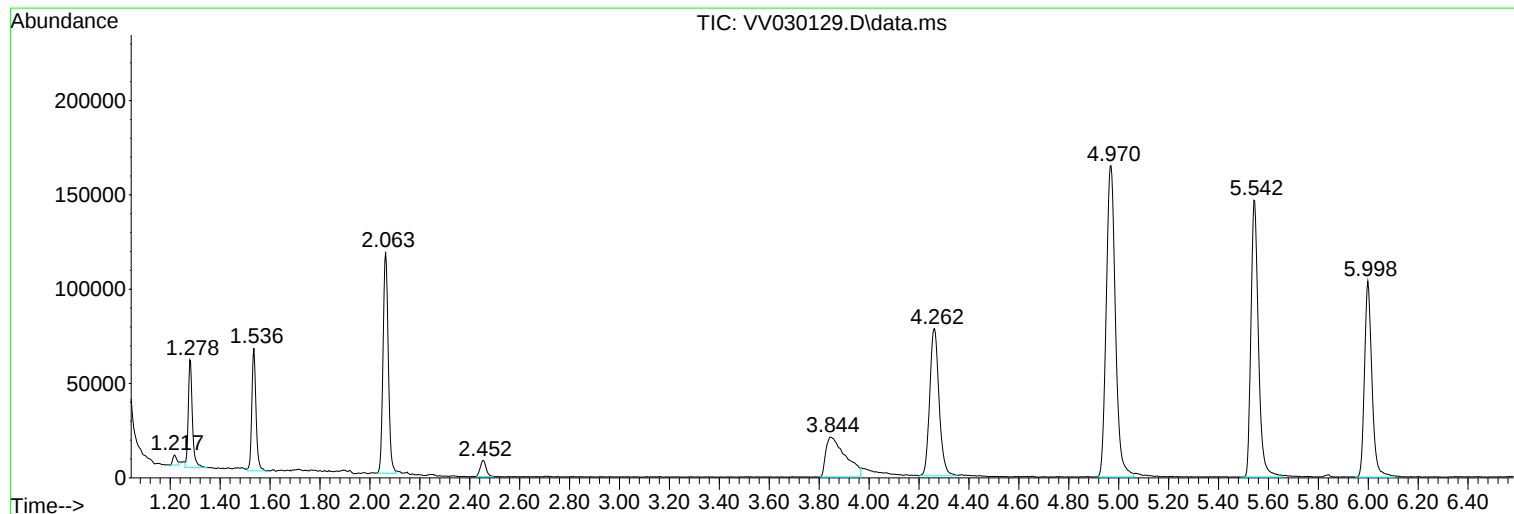

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
Data File : VV030129.D
Acq On : 03 Mar 2023 10:08
Operator : SY/MD
Sample : VV0303WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK307

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
Data File : VV030129.D
Acq On : 03 Mar 2023 10:08
Operator : SY/MD
Sample : VV0303WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK307

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc