

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
 Data File : VV030130.D
 Acq On : 03 Mar 2023 11:03
 Operator : SY/MD
 Sample : 01769-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBYL3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030130.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	51	56	61	rBV2	4157	4764	1.06%	0.125%
2	1.281	68	75	91	rVB	62035	70211	15.58%	1.847%
3	1.536	147	154	166	rVB	66769	76071	16.88%	2.001%
4	2.063	308	318	333	rBV	121027	176668	39.21%	4.648%
5	3.815	853	863	903	rBV	38211	144929	32.16%	3.813%
6	4.259	983	1001	1028	rBV2	84330	213203	47.32%	5.609%
7	4.966	1204	1221	1258	rBV2	175948	450583	100.00%	11.853%
8	5.542	1384	1400	1429	rBV	156019	322208	71.51%	8.476%
9	5.998	1529	1542	1563	rBV	107193	221830	49.23%	5.836%
10	6.921	1818	1829	1845	rBV	40206	75102	16.67%	1.976%
11	7.252	1917	1932	1950	rBV	199154	353594	78.47%	9.302%
12	7.326	1950	1955	1967	rVB2	4562	8133	1.80%	0.214%
13	7.561	2017	2028	2049	rBV2	23971	44015	9.77%	1.158%
14	8.034	2165	2175	2205	rBV	190036	364761	80.95%	9.596%
15	8.792	2400	2411	2435	rBV	235847	395539	87.78%	10.405%
16	8.956	2454	2462	2472	rVB2	5688	7919	1.76%	0.208%
17	10.162	2822	2837	2855	rBV	83792	132108	29.32%	3.475%
18	10.336	2882	2891	2901	rVB	5895	8827	1.96%	0.232%
19	11.194	3147	3158	3179	rBV	246366	382656	84.92%	10.067%
20	11.570	3262	3275	3295	rBV	209100	333871	74.10%	8.783%
21	13.693	3924	3935	3944	rBV3	9411	14276	3.17%	0.376%




Sum of corrected areas: 3801268

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
Data File : VV030130.D
Acq On : 03 Mar 2023 11:03
Operator : SY/MD
Sample : 01769-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBYL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

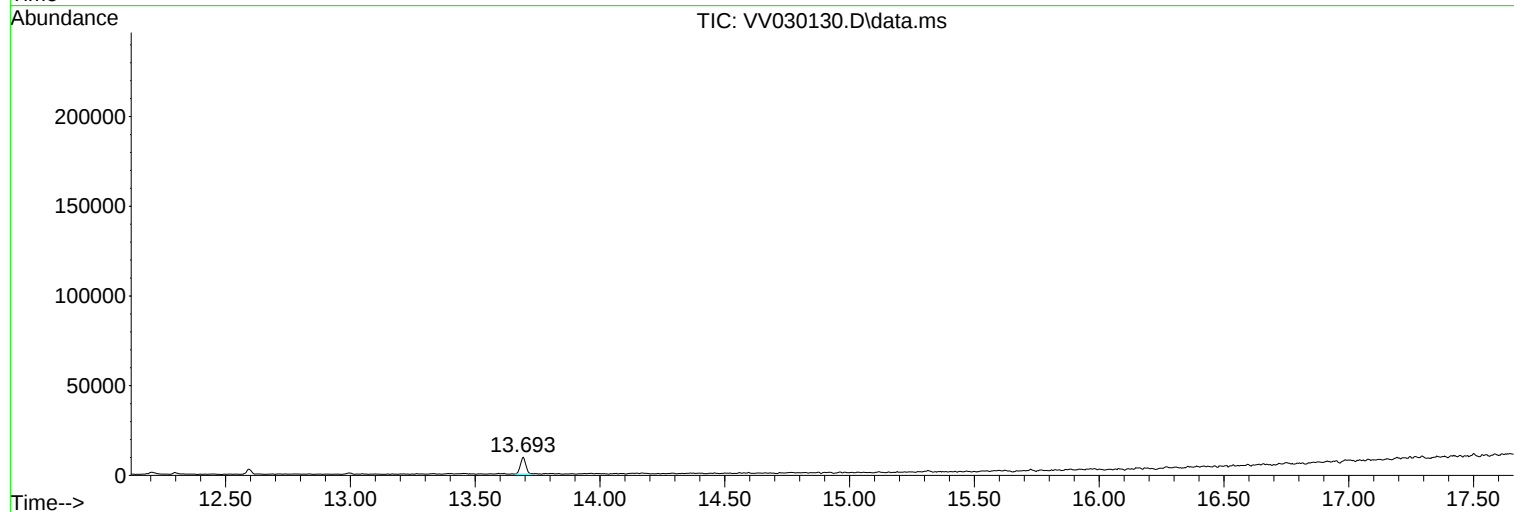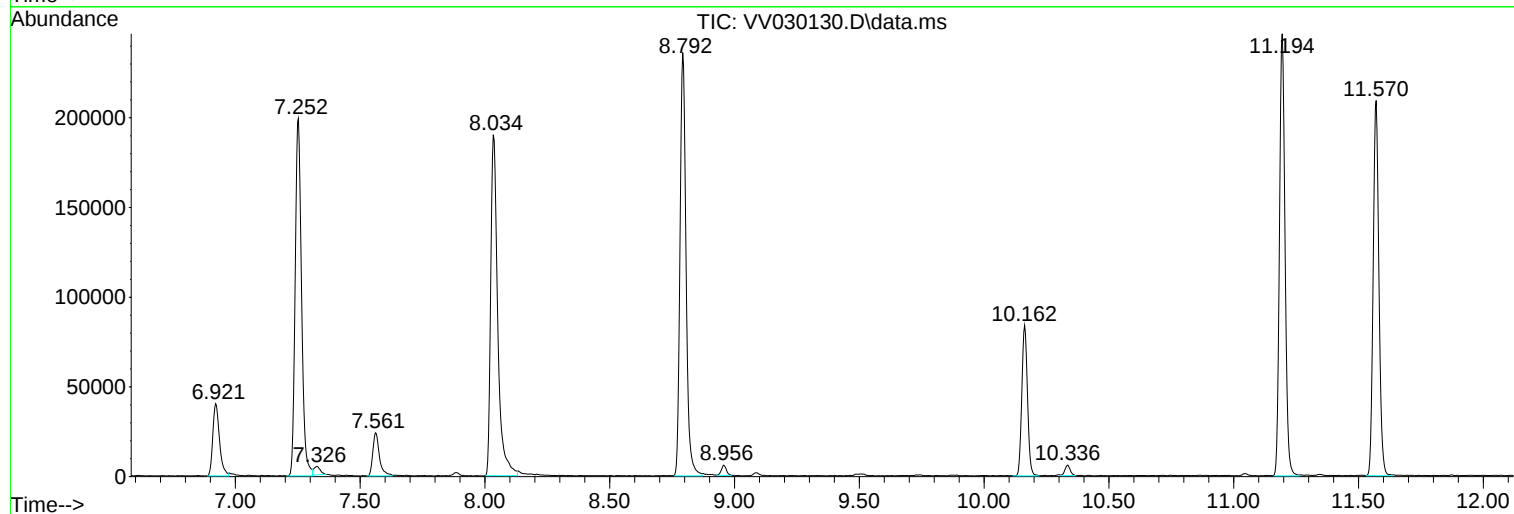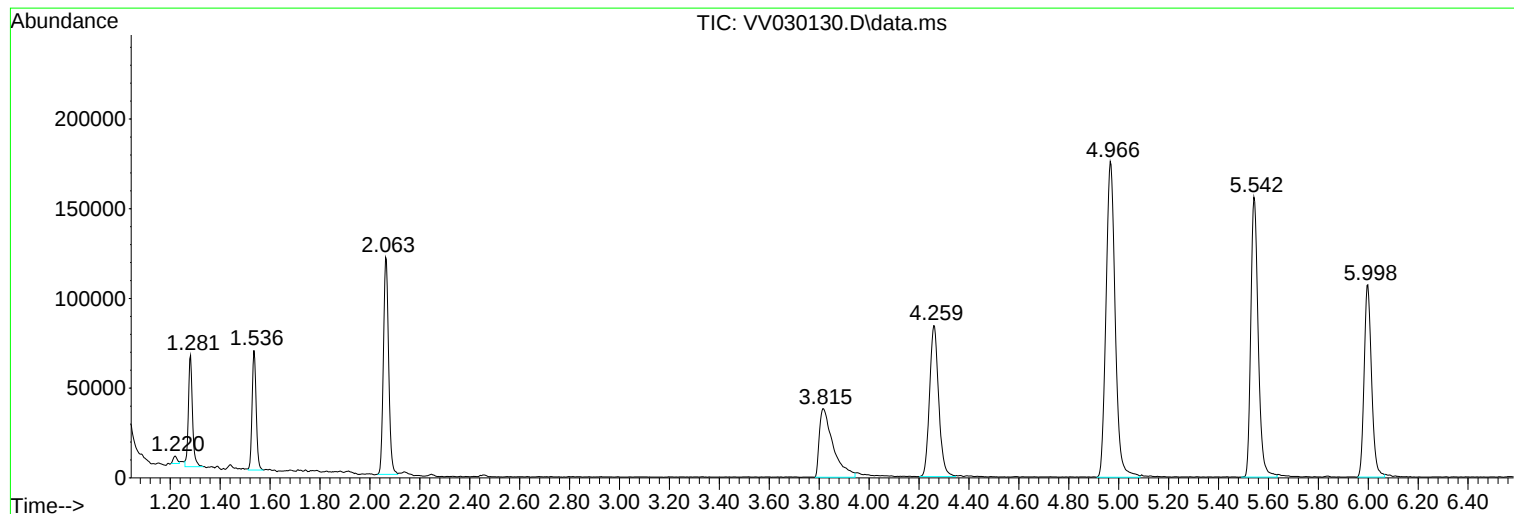

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
Data File : VV030130.D
Acq On : 03 Mar 2023 11:03
Operator : SY/MD
Sample : 01769-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBYL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
Data File : VV030130.D
Acq On : 03 Mar 2023 11:03
Operator : SY/MD
Sample : 01769-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBYL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc