

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
 Data File : VV030132.D
 Acq On : 03 Mar 2023 11:52
 Operator : SY/MD
 Sample : 01769-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBYL5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030132.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	52	56	66	rVV2	4659	5752	1.21%	0.143%
2	1.281	69	75	89	rVB	62634	70130	14.72%	1.746%
3	1.442	118	125	138	rBV	17077	19951	4.19%	0.497%
4	1.539	147	155	172	rVB	70029	82559	17.33%	2.056%
5	1.674	186	197	207	rBV	14056	18325	3.85%	0.456%
6	2.066	308	319	337	rBV	126198	185037	38.83%	4.608%
7	3.815	853	863	912	rBV	43230	162897	34.19%	4.056%
8	4.262	985	1002	1026	rBV2	86895	222567	46.71%	5.542%
9	4.969	1204	1222	1254	rBV2	186030	476475	100.00%	11.865%
10	5.545	1385	1401	1428	rBV	156065	325755	68.37%	8.112%
11	5.998	1528	1542	1568	rBV	112537	231832	48.66%	5.773%
12	6.921	1817	1829	1857	rBV2	42238	79815	16.75%	1.988%
13	7.252	1919	1932	1973	rBV	209194	377961	79.32%	9.412%
14	7.561	2019	2028	2048	rBV	24741	46200	9.70%	1.150%
15	7.882	2118	2128	2141	rVB3	5272	9617	2.02%	0.239%
16	8.037	2164	2176	2210	rBV	213354	400430	84.04%	9.971%
17	8.792	2400	2411	2437	rBV	240887	401283	84.22%	9.993%
18	10.162	2825	2837	2855	rBV2	91022	143317	30.08%	3.569%
19	10.336	2880	2891	2905	rVB2	14015	21982	4.61%	0.547%
20	11.194	3147	3158	3179	rBV	245598	386180	81.05%	9.617%
21	11.570	3263	3275	3292	rBV	218536	342318	71.84%	8.524%
22	12.207	3464	3473	3481	rVB2	3609	5363	1.13%	0.134%




Sum of corrected areas: 4015746

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
Data File : VV030132.D
Acq On : 03 Mar 2023 11:52
Operator : SY/MD
Sample : 01769-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBYL5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

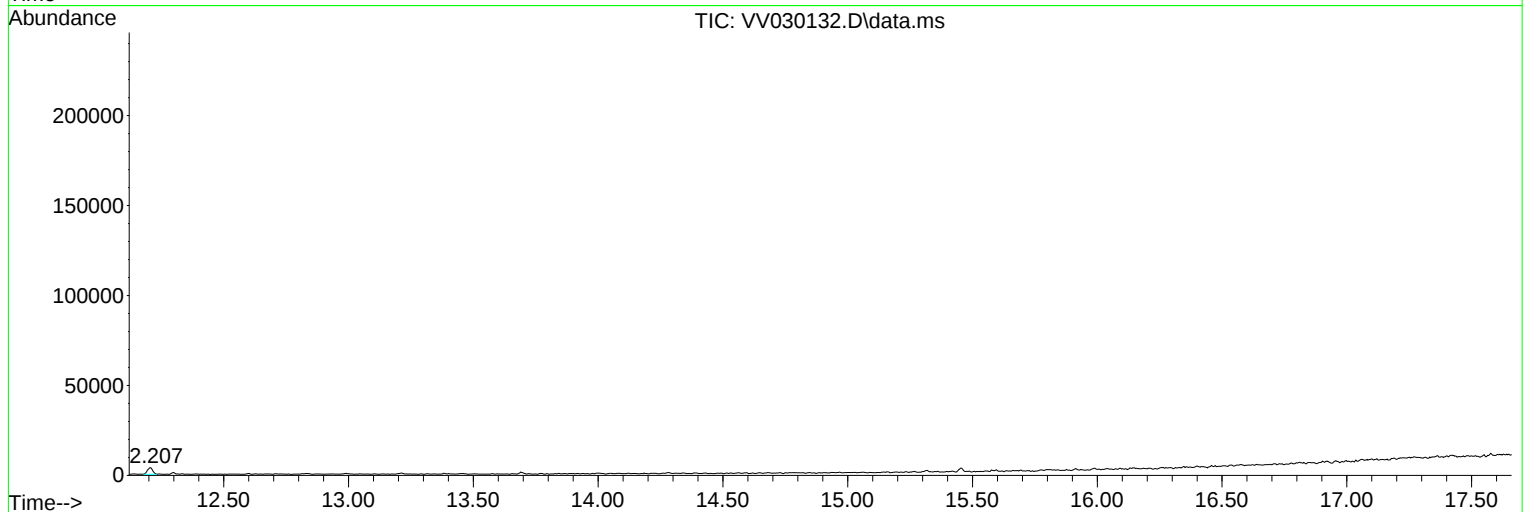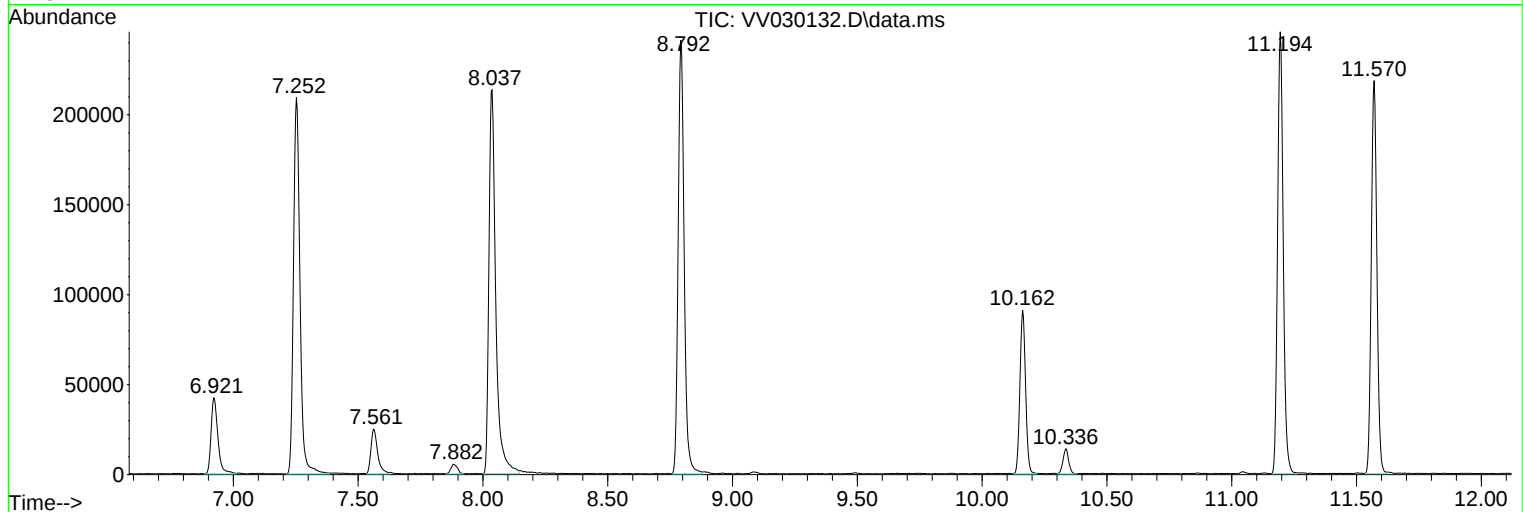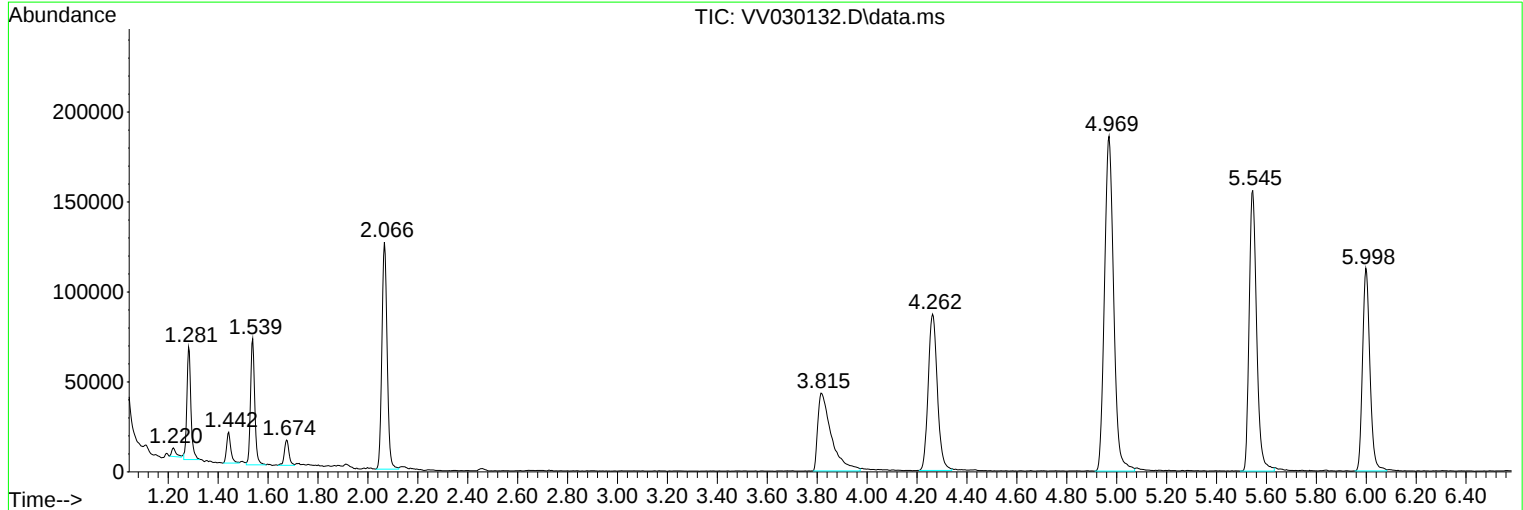

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
Data File : VV030132.D
Acq On : 03 Mar 2023 11:52
Operator : SY/MD
Sample : 01769-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBYL5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
Data File : VV030132.D
Acq On : 03 Mar 2023 11:52
Operator : SY/MD
Sample : 01769-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBYL5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------