

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
 Data File : VV030136.D
 Acq On : 03 Mar 2023 13:36
 Operator : SY/MD
 Sample : 01769-02DL 500X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBYL2DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030136.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	52	56	68	rVV2	4355	5703	1.37%	0.159%
2	1.282	69	75	92	rVB	54796	63484	15.24%	1.768%
3	1.536	147	154	171	rVB	60044	73040	17.53%	2.034%
4	2.066	308	319	335	rBV	111826	163647	39.28%	4.558%
5	2.175	337	353	357	rBV	10447	25874	6.21%	0.721%
6	2.458	431	441	452	rVB2	5004	8452	2.03%	0.235%
7	3.854	861	875	921	rBV2	21099	123680	29.69%	3.445%
8	4.265	986	1003	1029	rBV	78523	200086	48.03%	5.572%
9	4.969	1206	1222	1261	rBV2	161996	416567	100.00%	11.601%
10	5.545	1385	1401	1424	rBV	147831	307794	73.89%	8.572%
11	6.002	1524	1543	1578	rBV	98103	210277	50.48%	5.856%
12	6.924	1819	1830	1852	rBV2	38434	72026	17.29%	2.006%
13	7.252	1920	1932	1955	rBV	177330	320365	76.91%	8.922%
14	7.564	2017	2029	2051	rBV	23399	42736	10.26%	1.190%
15	8.040	2163	2177	2220	rBV	174556	368902	88.56%	10.274%
16	8.792	2399	2411	2441	rBV	228140	383254	92.00%	10.674%
17	10.162	2826	2837	2858	rBV	82461	131154	31.48%	3.653%
18	11.194	3147	3158	3185	rBV	235109	360070	86.44%	10.028%
19	11.570	3261	3275	3294	rBV	190719	299040	71.79%	8.328%
20	12.204	3454	3472	3483	rBV	5150	8091	1.94%	0.225%
21	13.995	4015	4029	4040	rBV2	3490	6389	1.53%	0.178%




Sum of corrected areas: 3590631

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
Data File : VV030136.D
Acq On : 03 Mar 2023 13:36
Operator : SY/MD
Sample : 01769-02DL 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBYL2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

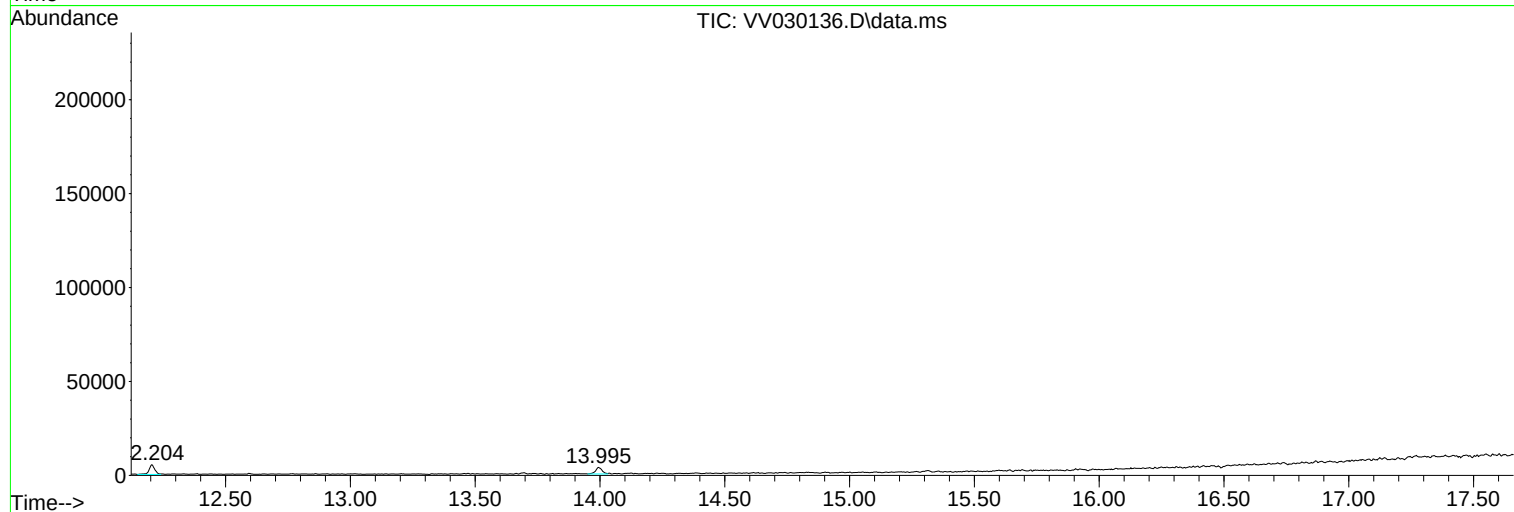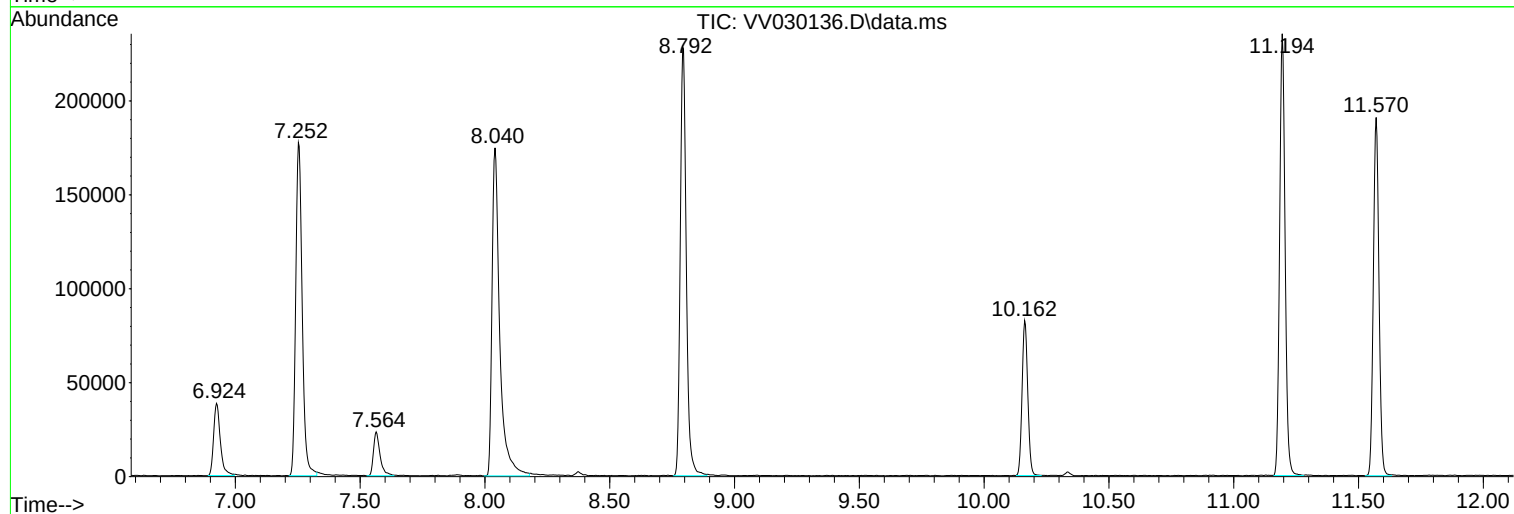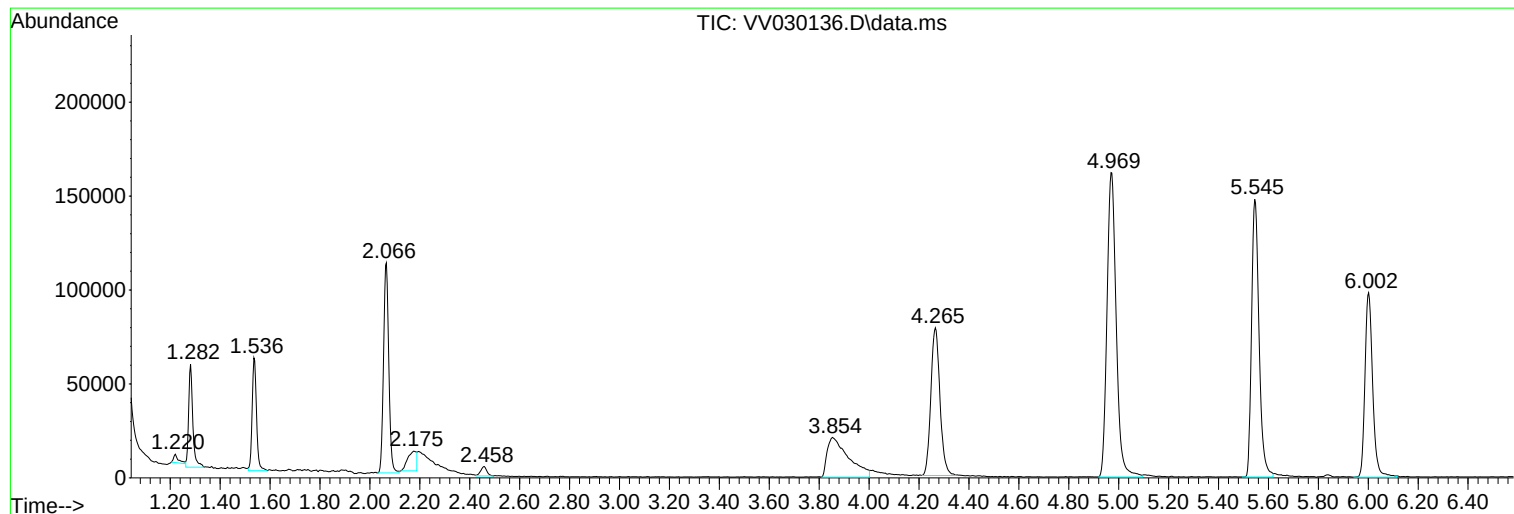

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
Data File : VV030136.D
Acq On : 03 Mar 2023 13:36
Operator : SY/MD
Sample : 01769-02DL 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBYL2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
Data File : VV030136.D
Acq On : 03 Mar 2023 13:36
Operator : SY/MD
Sample : 01769-02DL 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBYL2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------